
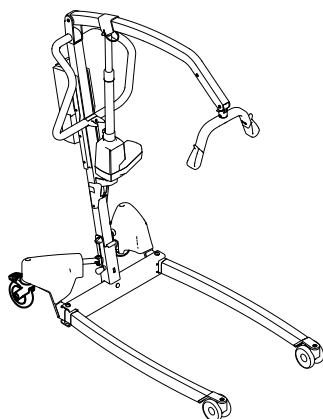
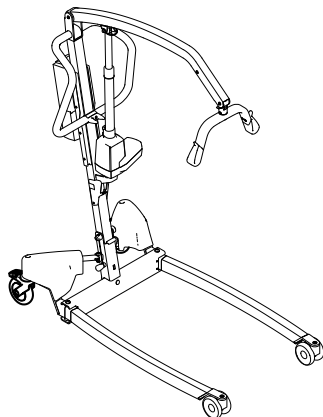
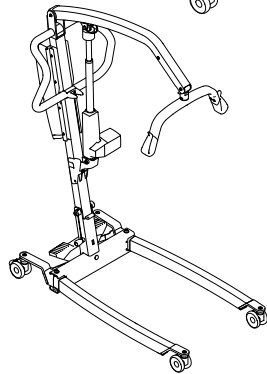


Invacare® Birdie® EVO

Birdie® EVO, Birdie® EVO COMPACT, Birdie® EVO PLUS,
Birdie® EVO XPLUS

en Mobile Patient Lift Service Manual

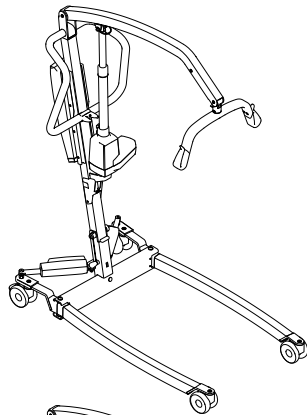

PROVIDER: Keep this manual.
The procedures in this manual MUST be performed by a qualified technician.



Yes, you can.®

Contents

| | |
|---|-----------|
| 1 General | 4 |
| 1.1 Introduction | 4 |
| 1.1.1 Symbols in this Document | 4 |
| 2 Safety | 5 |
| 2.1 General Safety Information | 5 |
| 2.2 Main parts of the lift. | 5 |
| 3 Servicing | 6 |
| 3.1 Service Interval | 6 |
| 3.1.1 LOLER Statement | 6 |
| 3.2 Tightening torques | 6 |
| 3.3 Resetting the service light | 6 |
| 3.4 Service inspection checklist | 7 |
| 4 Troubleshooting | 9 |
| 4.1 Identifying and repairing faults | 9 |
| 5 Instructions | 11 |
| 5.1 Disassembling a foldable mast | 11 |
| 5.2 Assembling a foldable mast | 11 |
| 5.3 Replacing 75 mm castors | 12 |
| 5.4 Replacing 100 mm castors | 12 |
| 5.5 Replacing 100 mm rear castors with total lock | 13 |
| 5.6 Replacing 125 mm castors | 14 |
| 5.7 Replacing the spreader bar | 15 |
| 5.8 Replacing the hooks | 15 |
| 5.9 Replacing the boom actuator | 16 |
| 5.10 Replacing the boom | 17 |
| 5.11 Replacing the damper | 17 |
| 5.12 Replacing a leg actuator without cover | 18 |
| 5.13 Replacing a leg actuator with cover | 19 |
| 5.14 Replacing electrical legs without actuator cover | 21 |
| 5.15 Replacing electrical legs with actuator cover | 22 |
| 5.16 Replacing the foot pedal and/or rods | 23 |
| 5.17 Replacing manual legs | 24 |
| 5.18 Replacing the CBJ Home control unit | 25 |
| 5.19 Replacing the CBJ Care, CBJ1 , CBJ2 control unit | 26 |
| 5.20 Installing the Wunder RS300 scale with SMARTLOCK® | 27 |
| 5.21 Installing the Wunder RS300 scale with a fixed spreader bar | 28 |
| 5.22 Installing the Wunder CR200 scale with SMARTLOCK® | 29 |
| 5.23 Installing the Wunder CR200 scale with a fixed spreader bar | 30 |
| 5.24 Installing the lever for manual leg spreader | 31 |

1 General

1.1 Introduction

This document contains important information about assembly, adjustment and advanced maintenance of the product. To ensure safety when handling the product, read this document and the user manual carefully and follow the safety instructions.

Find the user manual on Invacare's website or contact your Invacare representative. See addresses at the end of this document.

Invacare reserves the right to alter product specifications without further notice.

Before reading this document, make sure you have the latest version. You find the latest version as a PDF on the Invacare website.

For pre-sale and user information, see the user manual.

For more information about the product, for example product safety notices and product recalls, contact your Invacare representative. See addresses at the end of this document.

1.1.1 Symbols in this Document

Symbols and signal words are used in this document and apply to hazards or unsafe practices which could result in personal injury or property damage. See the information below for definitions of the signal words.



WARNING

Indicates a hazardous situation that could result in serious injury or death if it is not avoided.



CAUTION

Indicates a hazardous situation that could result in minor or slight injury if it is not avoided.



IMPORTANT

Indicates a hazardous situation that could result in damage to property if it is not avoided.



Tips and Recommendations

Gives useful tips, recommendations and information for efficient, trouble-free use.

2 Safety

2.1 General Safety Information


WARNING!
Risk of injury or damage to property

- The procedures in this manual must only be performed by a qualified technician.
- Use only original accessories and spare parts.
- Do not handle this product or any available optional equipment without first completely reading and understanding these instructions and any additional instructional material such as user manuals, installation manuals or instruction sheets supplied with this product or optional equipment.
- After each assembly, check that all fittings are properly tightened and that all parts have the correct function.


WARNING!
Risk of contamination

- Clean and disinfect the product before servicing.


IMPORTANT!

Assembly of accessories might not be described in this service manual. Refer to the manual, delivered with the accessory.

- Additional manuals can be ordered from Invacare. See addresses at the end of this document.


IMPORTANT!

Some replacement parts are only available as a kit. Always use the complete new kit when replacing a part.

- Spare parts can be ordered from Invacare. Refer to your local Invacare website to access the electronic spare parts catalogue (ESPC).


IMPORTANT!


Refer to the user manual of this product for information on

- Technical data
- Product components
- Labels
- Additional safety instructions
- Cleaning and disinfection instructions



The information contained in this document is subject to change without notice.

2.2 Main parts of the lift

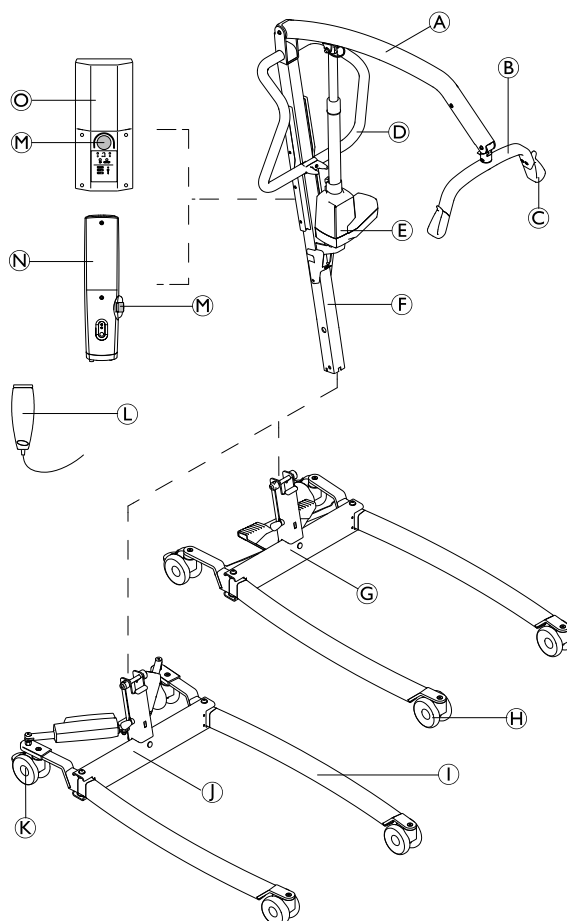

| | |
|-----|---|
| (A) | Boom |
| (B) | Spreader bar – with or without SMARTLOCK™ |
| (C) | Hook for sling |
| (D) | Push bar |
| (E) | Lifting actuator |
| (F) | Mast – foldable or fixed |
| (G) | Base with foot pedal for manual leg spreader |
| (H) | Front Castors |
| (I) | Leg |
| (J) | Base with actuators for electrical leg spreader – with or without actuator covers |
| (K) | Rear castors with brake |
| (L) | Hand control |
| (M) | Emergency Stop |
| (N) | CBJ Home control unit with integrated battery |
| (O) | CBJ Care, CBJ1 or CBJ2 control unit with detachable battery |

3 Servicing

3.1 Service Interval

Unless otherwise stated in local requirements, service must be performed at least every 12 months and according to the Service Inspection Checklist. When performing annual or regular service, all parts designed to carry load must be, as a minimum, tested with maximum load. All safety features must be checked according to ISO 10535:2006 Annex B.

3.1.1 LOLER Statement

The UK Health and Safety Executive's Lifting Operations and Lifting Equipment Regulations 1998, require any equipment that is used in the workplace to lift a load be subject to safety inspection on a six monthly basis. Please refer to the HSE web site for guidance www.hse.gov.uk.

The person responsible for the equipment must ensure adherence to LOLER regulations.

3.2 Tightening torques



IMPORTANT

Do not overtighten the mounting hardware as this might cause damage to the product.

If not otherwise stated in the specific instructions the following guidelines apply:

| Thread | Tightening torque in Nm \pm 10% |
|--------|-----------------------------------|
| M4 | 3 Nm |
| M5 | 6 Nm |
| M6 | 10 Nm |
| M8 | 25 Nm |
| M10 | 49 Nm |
| M12 | 80 Nm |
| M16 | 180 Nm |

3.3 Resetting the service light

(CBJ Care control unit only)


To reset the service light after a service has been performed:

1. Locate the hand control.
2. Press and hold the UP button and the DOWN button at the same time for five seconds.
3. You will hear a sound when the service light has been reset.


The service light is now reset to indicate a service requirement after a 12 month period or 8000 cycles.

If the service light is required to be set for a period shorter than 12 months, a special handset and further instructions are required. Contact Invacare to order this handset and instructions.

3.4 Service inspection checklist

| | | | |
|---|--------|------------------|-----|
|  | Model: | REF / SN number: | 1/2 |
|---|--------|------------------|-----|

| Checkpoints for Invacare® Birdie® EVO according to ISO 10535:2006 Annex B | ✓ | ✗ | Comment |
|---|---|---|---------|
| General inspection | | | |
| No unauthorized modifications | | | |
| All labels present and readable. (see full list of labels in the user manual) | | | |
| Safe working load visibly marked on product label and boom | | | |
| User manual available | | | |
| Visual inspection of mechanical parts | | | |
| No wear and deformation on pivot points and bolts (leg-base connection, mast-boom connection, actuator attachments) | | | |
| All connecting elements (screws and bolts) present and properly tightened or secured | | | |
| No deformation, cracks or other damages on welded joints | | | |
| Surfaces free of damages and corrosion | | | |
| No deformation on metal structure (legs, base, mast, boom and spreader bar) | | | |
| No deformation, wear, sharp edges or other damages on the sling hooks | | | |
| No deformation or other damages on spreader bar holder, leg spreader lever and spreader bar release mechanism (SMARTLOCK® option) | | | |
| Castors free of damages, debris and dirt | | | |
| Visual inspection of electrical parts | | | |
| All cables undamaged and routed properly | | | |
| No leakage on the actuator(s) | | | |
| No cracks or other damages on housings (actuators, control unit, hand control) | | | |

| | | | |
|---|--------|------------------|-----|
|  | Model: | REF / SN number: | 2/2 |
|---|--------|------------------|-----|

| Checkpoints for Invacare® Birdie® EVO according to ISO 10535:2006 Annex B | ✓ | ✗ | Comment |
|--|---|---|---------|
| Functional tests | | | |
| Castors smoothly swivel and roll | | | |
| Application and release of castor brakes is working properly | | | |
| Base fully opens and closes smoothly | | | |
| Emergency stop engages when pressed in and all electrical functions are disabled | | | |
| Emergency stop can be reset when button is turned clockwise | | | |
| Emergency functions on the control unit (emergency lowering and if applicable emergency lifting) are working properly | | | |
| Mechanical emergency lowering lowers the boom at safe speed | | | |
| Successful load test (full lifting cycle with maximum safe working load applied) with quiet and smooth operation of the actuator | | | |
| All buttons on the control unit and hand control are working and activate the correct function | | | |
| Battery indicator and LEDs on the control unit are working properly | | | |
| Release mechanism of the spreader bar is working properly (release, smooth removal/insertion and self-locking) (SMARTLOCK® option) | | | |
| Dampening mechanism of the spreader bar is working properly (smooth swinging, effective dampening) (Slow'R® option) | | | |
| Folding mechanism of the mast is working properly (release, smooth folding/unfolding and self-locking) (option) | | | |

Overall assessment

| | |
|---|--|
| <input type="checkbox"/> Pass No safety or functional deficiencies were detected. | <input type="checkbox"/> Fail Safety or functional deficiencies detected and corrective action is required. Comments: |
|---|--|

Date of next inspection: _____

Name: _____ Date / Signature: _____

**IMPORTANT**

Corrective actions must be performed by a qualified technician.
 Instructions for replacing and adjusting main parts are described in the service manual.

4 Troubleshooting

4.1 Identifying and repairing faults

| Symptoms | Faults | Solution |
|--|---|--|
| Patient lift feels loose. | Mast/Base joint loose. | Check and tighten the Mast/ Base connection. See "Installing the Mast" in the user manual or 5.1 <i>Disassembling a foldable mast, page 11</i> |
| | Mast/Boom joint loose. | Check and tighten the Mast/ Boom connection. See 5.10 <i>Replacing the boom, page 17</i> |
| | Tie - Rods are loose. | Check and tighten the screws of the rods and/ or pedal. See 5.16 <i>Replacing the foot pedal and/or rods, page 23</i> |
| Castors/Brakes noisy or stiff. | Fluff or debris in bearings. | Replace the castors. See 5.3 <i>Replacing 75 mm castors, page 12</i> or 5.4 <i>Replacing 100 mm castors, page 12</i> |
| Noisy or dry sound from pivots. | Pivots are worn or damaged | Replace the pivots. See 5.10 <i>Replacing the boom, page 17</i> , 5.17 <i>Replacing manual legs, page 24</i> , 5.14 <i>Replacing electrical legs without actuator cover, page 21</i> or 5.15 <i>Replacing electrical legs with actuator cover, page 22</i> |
| Electric actuator fails to lift or legs fail to open when button is pressed. | Hand-control or actuator connector loose. | Connect hand control or actuator connector. Ensure connectors are seated properly and fully connected. |
| | Battery low. | Charge batteries. See "Charging the battery" in the user manual |
| | RED emergency stop button pressed IN. | Rotate RED emergency stop button CLOCKWISE until it pops out. |
| | Battery not connected properly to control unit. | Reconnect the battery to the control unit. See "Charging the battery" in the user manual |
| | The connecting terminals are damaged. | Replace the hand control and/or control unit. See 5.18 <i>Replacing the CBJ Home control unit, page 25</i> or 5.19 <i>Replacing the CBJ Care, CBJ1 , CBJ2 control unit, page 26</i> |
| | Power cord connected to power outlet. | Disconnect power cord from power outlet. |
| | Boom or leg actuator is worn or damaged or spindle is bent. | Replace the actuator. See 5.9 <i>Replacing the boom actuator, page 16</i> , 5.12 <i>Replacing a leg actuator without cover, page 18</i> or 5.13 <i>Replacing a leg actuator with cover, page 19</i> |
| Unusual noise from actuator. | Boom or leg actuator is worn or damaged or spindle is bent. | Replace the actuator. See 5.9 <i>Replacing the boom actuator, page 16</i> , 5.12 <i>Replacing a leg actuator without cover, page 18</i> or 5.13 <i>Replacing a leg actuator with cover, page 19</i> |
| Boom will not lower in uppermost position. | Boom requires a minimum weight load to lower from the uppermost position. | Pull down slightly on the boom. |
| Boom will not lower during a power retraction. | Shoulder bolt at the junction of the boom and mast may not be properly installed. | Check Mast/ Boom connection. See 5.10 <i>Replacing the boom, page 17</i> |

| Symptoms | Faults | Solution |
|---|-------------------------------------|---|
| The control unit emits a beeping sound during lifting, and the motor stops. | Max. load is exceeded | Reduce the load (and the lift will function normally). |
| Manual legs fail to open with the pedal or lever. | The mechanical mechanism is damaged | Replace foot pedal and/or rods. See <i>5.16 Replacing the foot pedal and/or rods, page 23</i> |
| Damping of the spreader bar has lessened or disappeared completely. | Damper is damaged | Replace the damper. See <i>5.11 Replacing the damper, page 17</i> |
| The detachable spreader bar does not fix to the connector on the boom | The locking mechanism is damaged | Replace the spreader bar connector. See <i>5.11 Replacing the damper, page 17</i> |

 Contact your Invacare provider or representative if the above does not solve your problems.

5 Instructions


5.1 Disassembling a foldable mast


CAUTION!
Risk of injury and damage to property

Improper handling of heavy parts can cause injury or damage to property.


- Always perform the following procedures with the mast in folded position.
- Assistance may be required to handle heavy parts.

1.

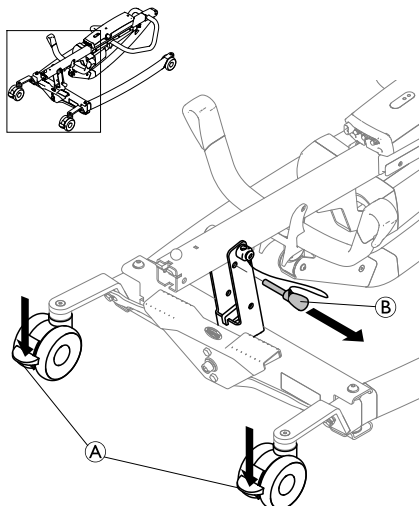


Lock both rear castors **A** and remove the locking pin **B**.

2.

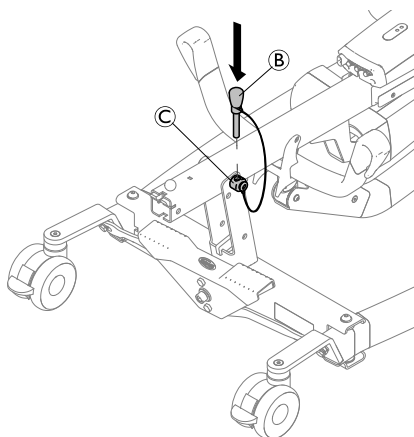


Insert the locking pin **B** into the hole on the pivot pin **C**.

3.

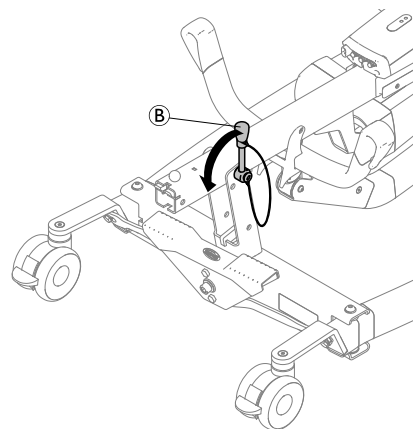


Rotate the locking pin **B** anti-clockwise to unlock the pivot pin **C**.

4.

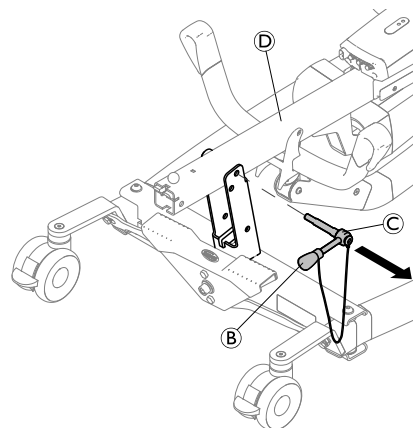

Hold the mast-boom assembly **D** in position and remove the pivot pin **C** with the locking pin **B**.

5.

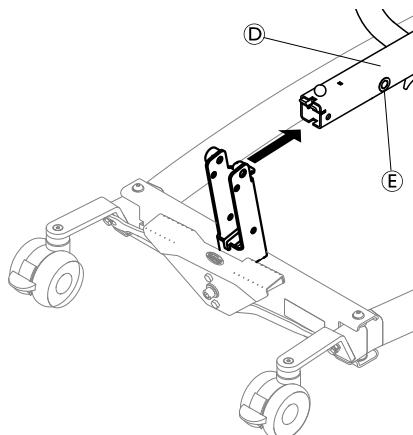

Remove the mast-boom assembly **D** from the base.




The bushings **E** are not fixed to the mast. Store them in a safe place or fix them to the mast with tape during transport and storage.


5.2 Assembling a foldable mast

1. Reverse the procedure described in *5.1 Disassembling a foldable mast, page 11*.
2. Check that the pivot pin is completely inserted and properly secured.
3. The mast can now be folded upright for usage.




5.3 Replacing 75 mm castors

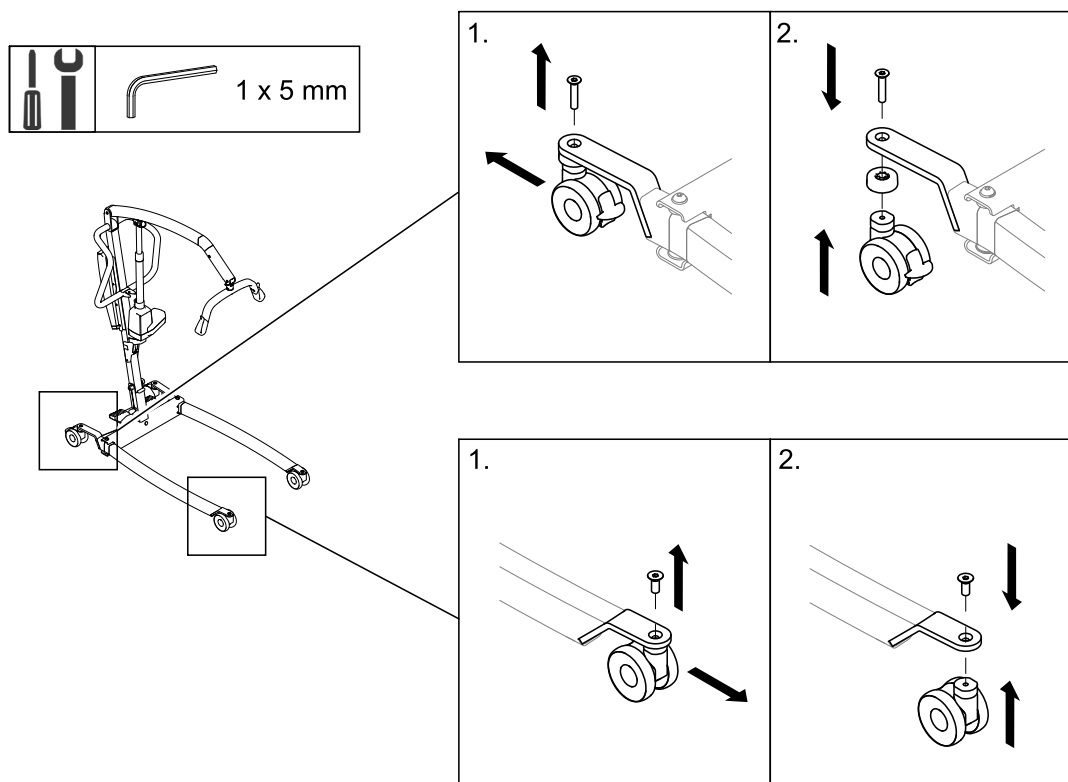







5.4 Replacing 100 mm castors

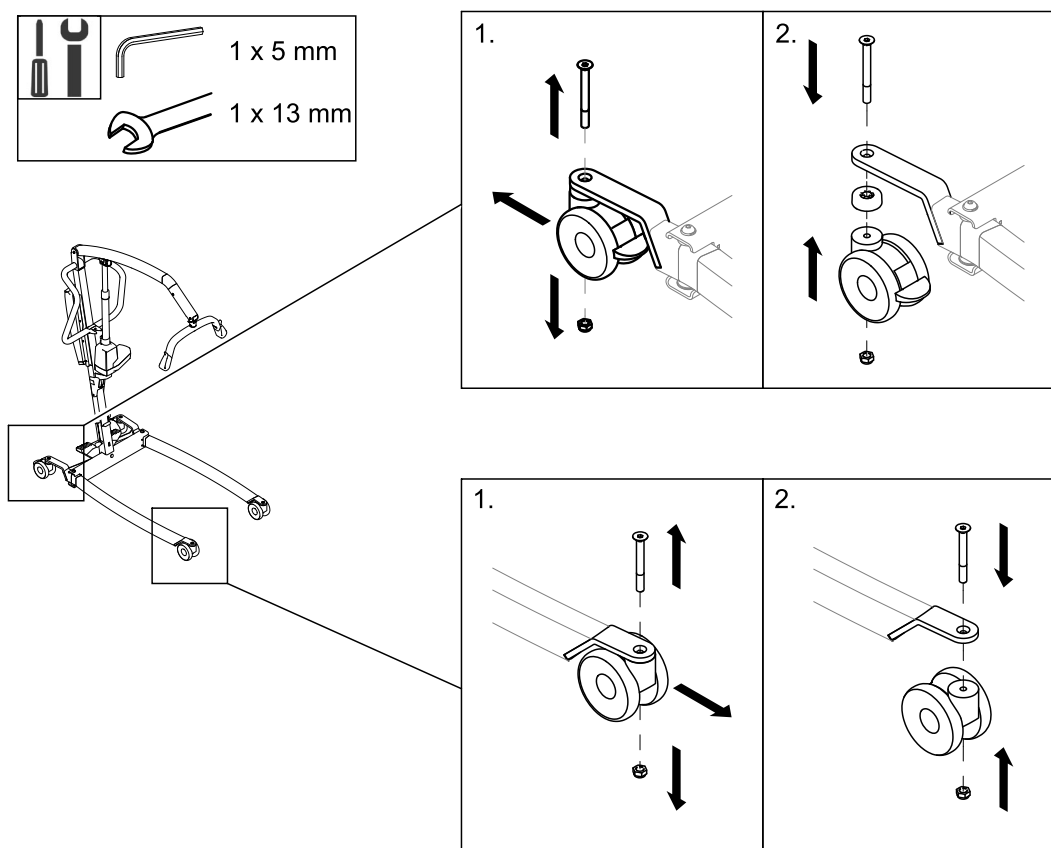




5.5 Replacing 100 mm rear castors with total lock

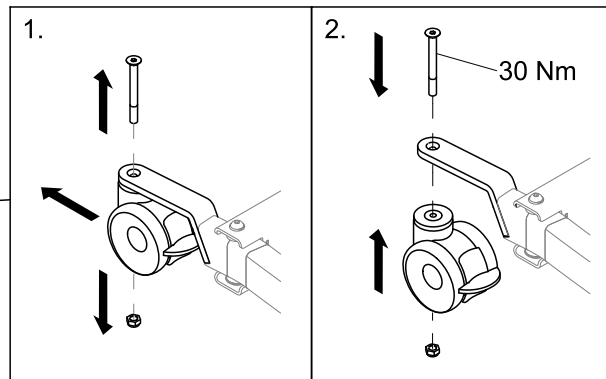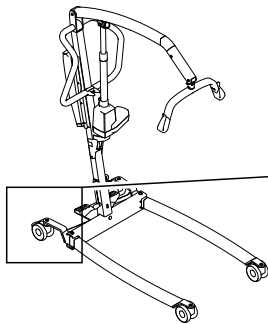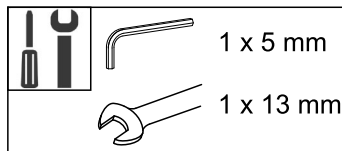




5.6 Replacing 125 mm castors

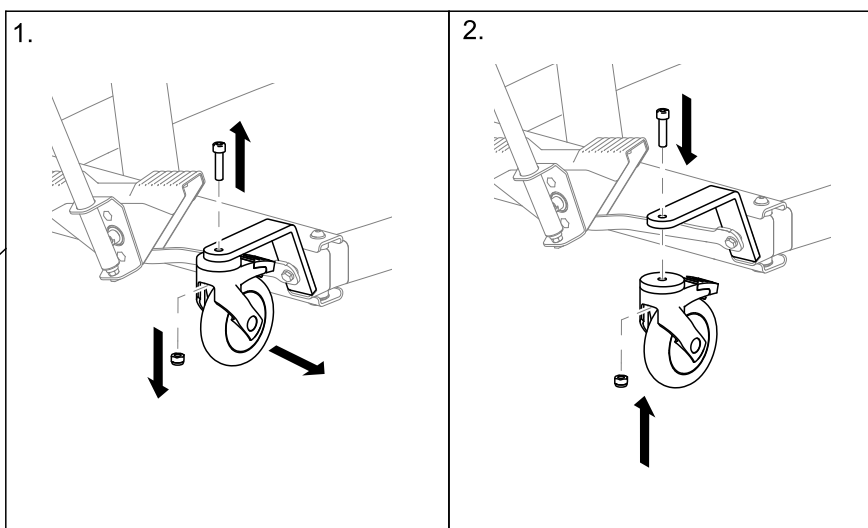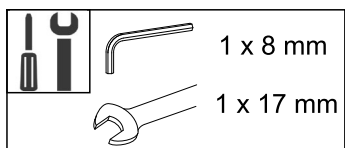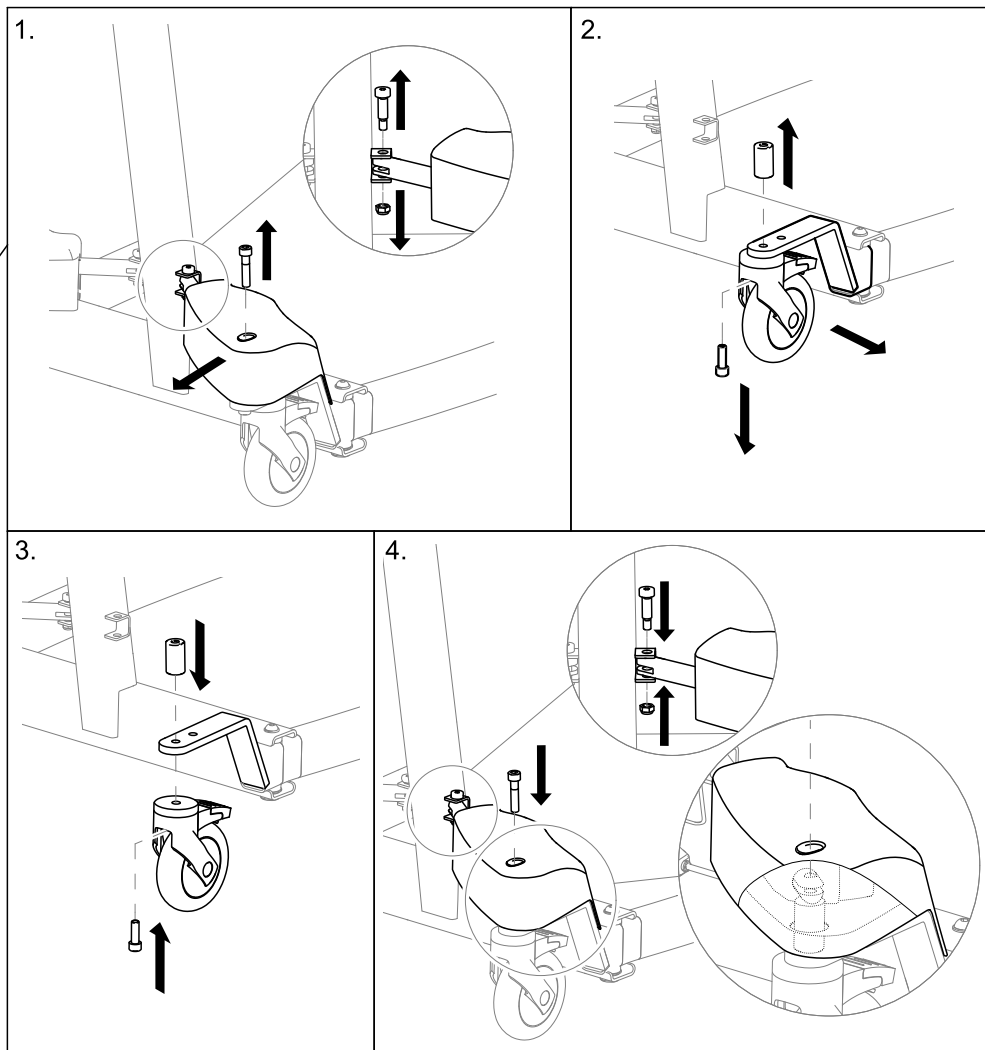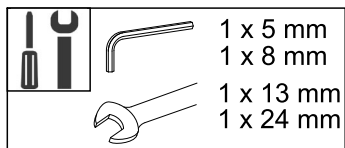




5.7 Replacing the spreader bar

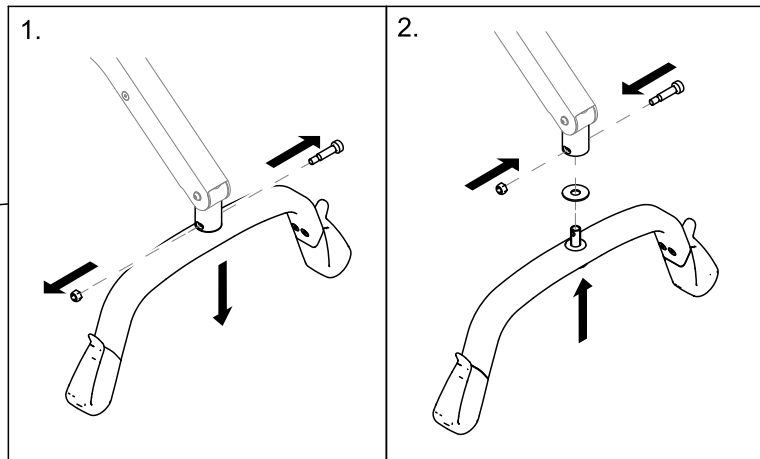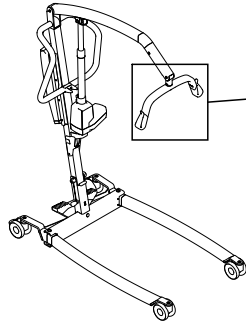




5.8 Replacing the hooks

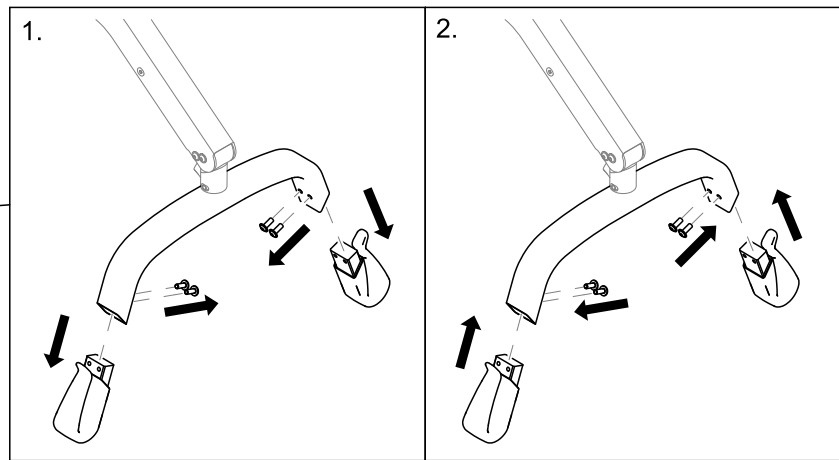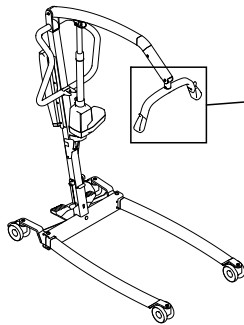




5.9 Replacing the boom actuator

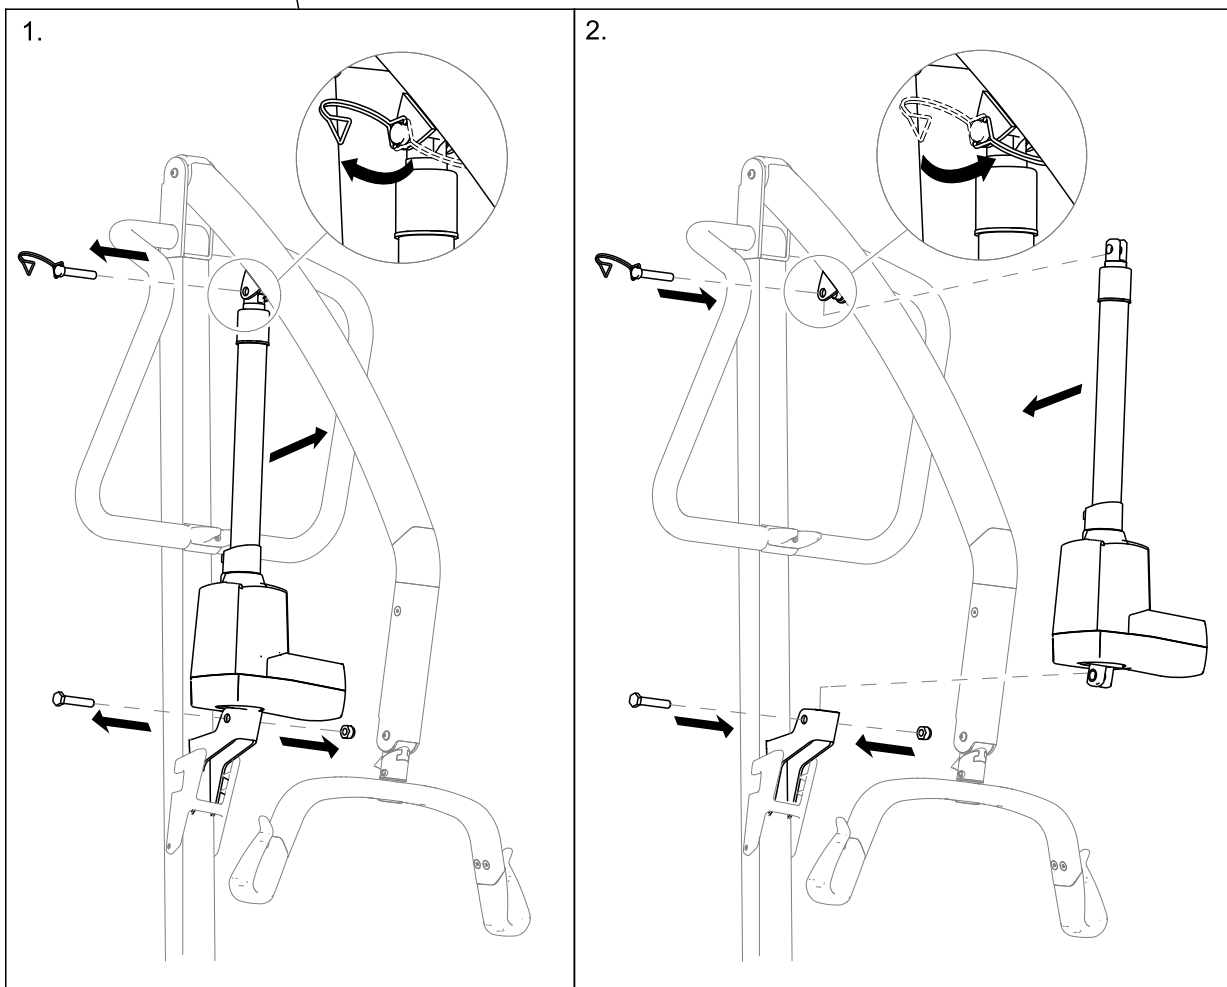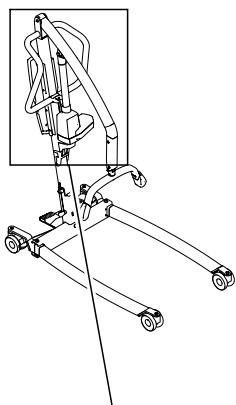




5.10 Replacing the boom

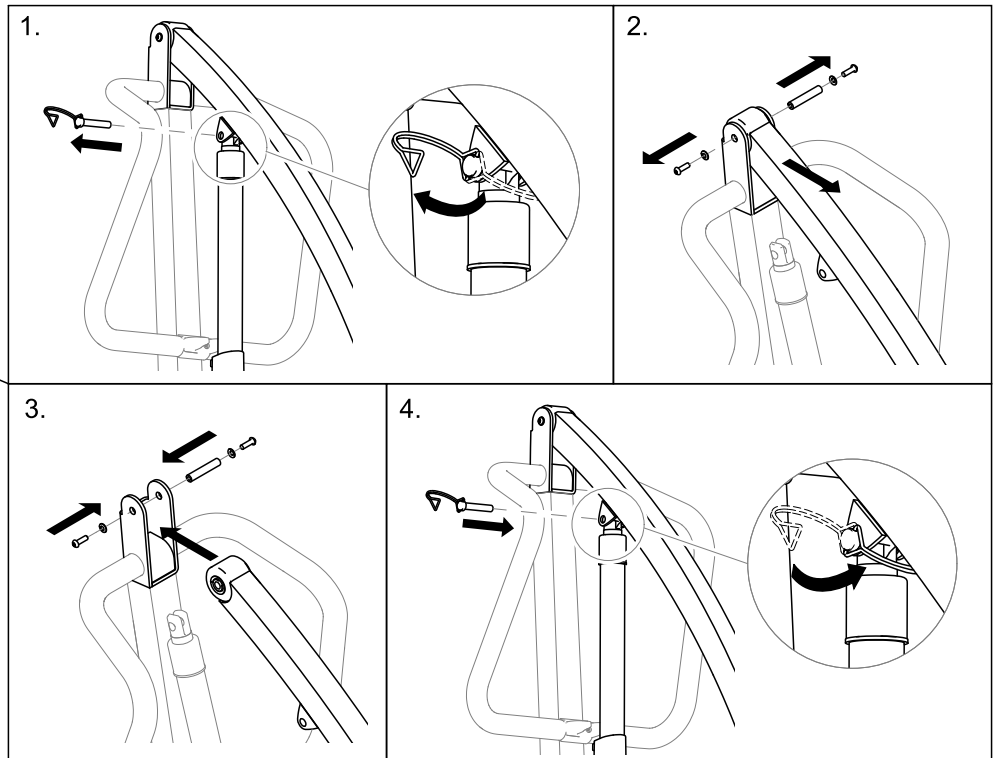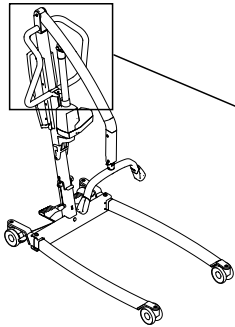


5.11 Replacing the damper

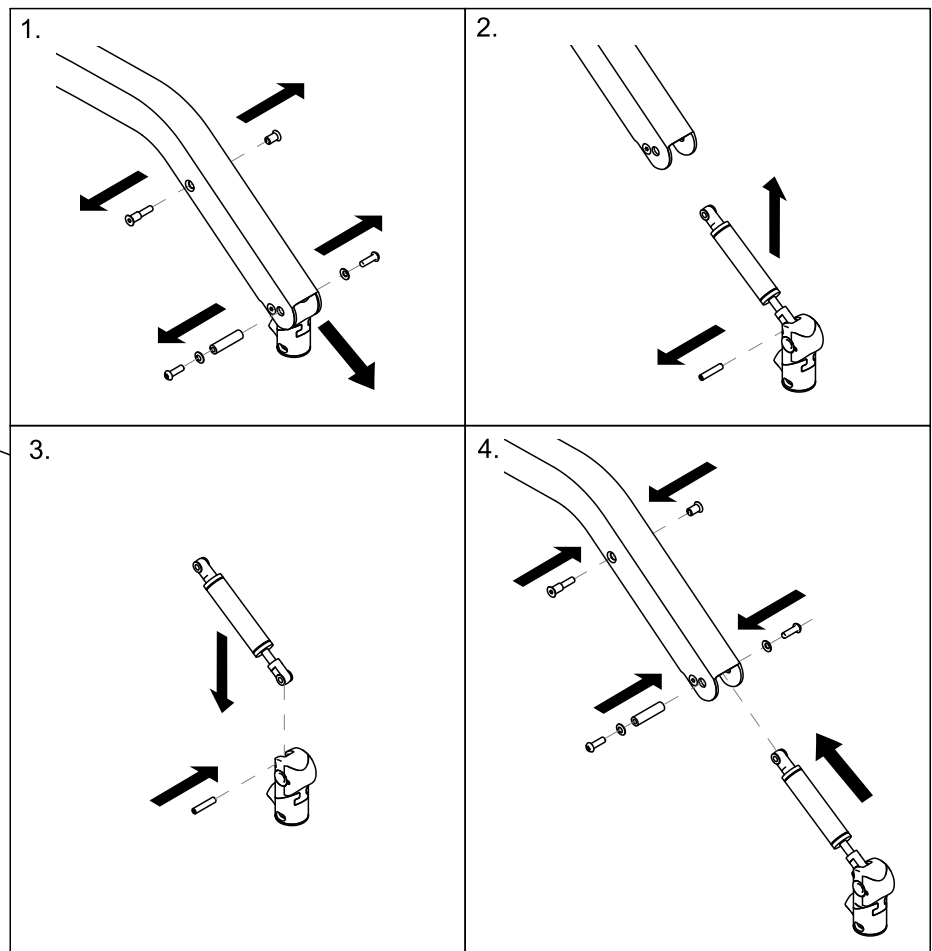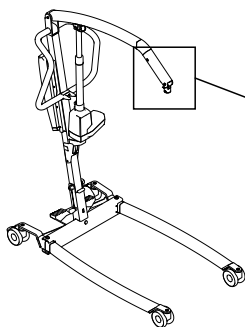


5.12 Replacing a leg actuator without cover

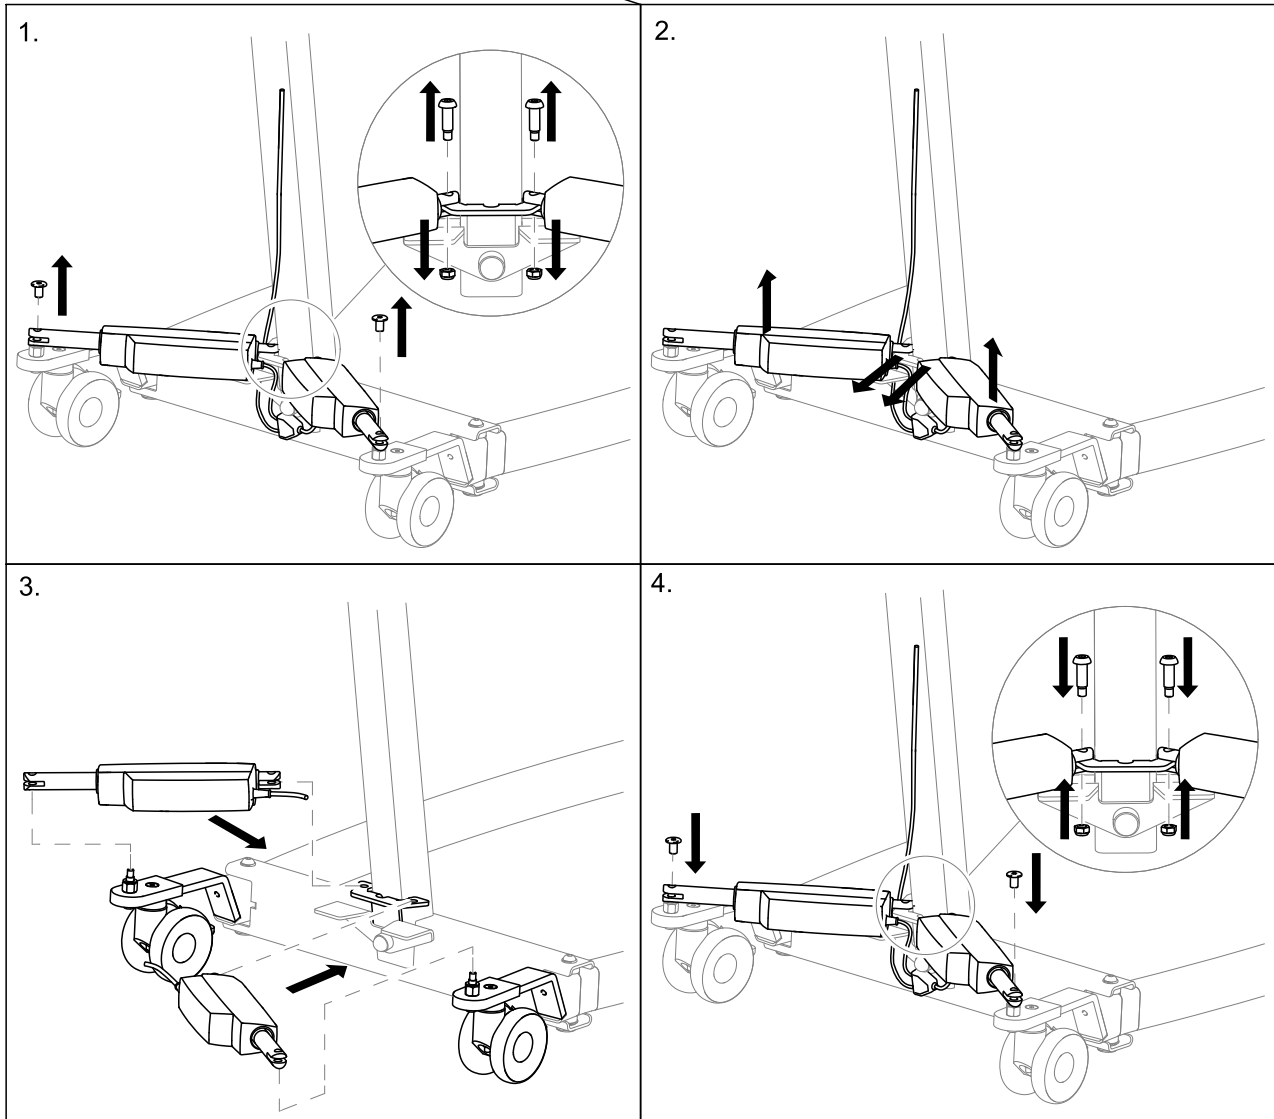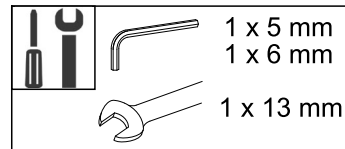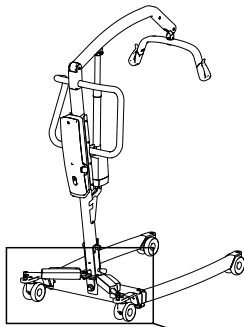


5.13 Replacing a leg actuator with cover

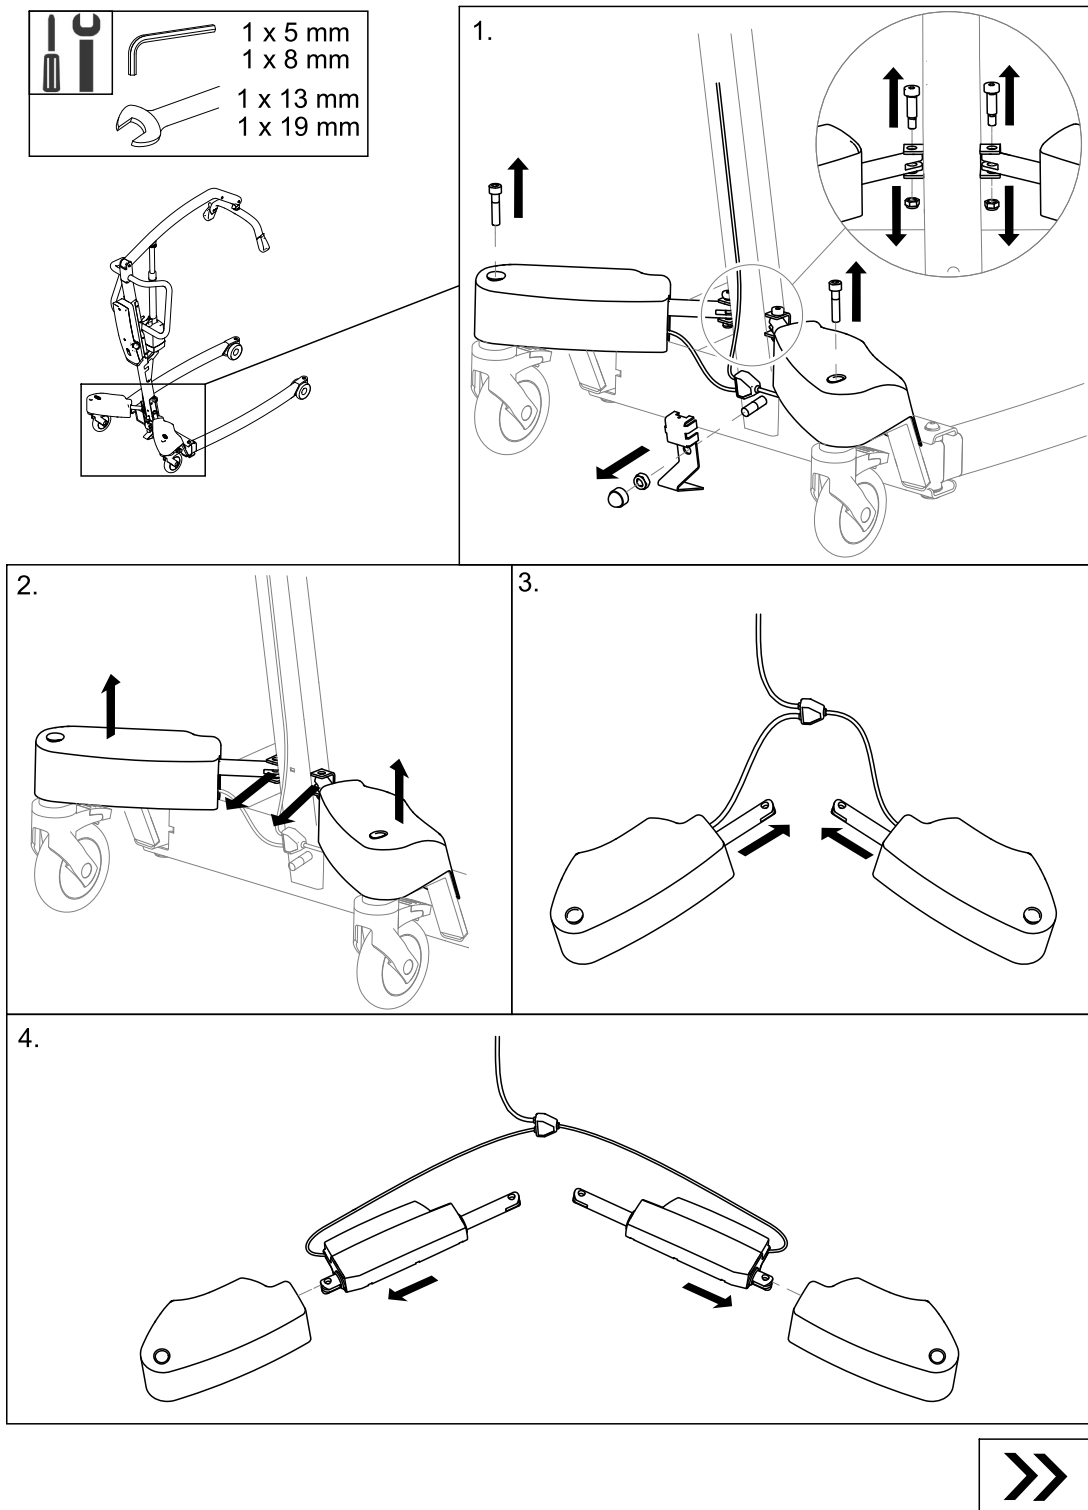









5.

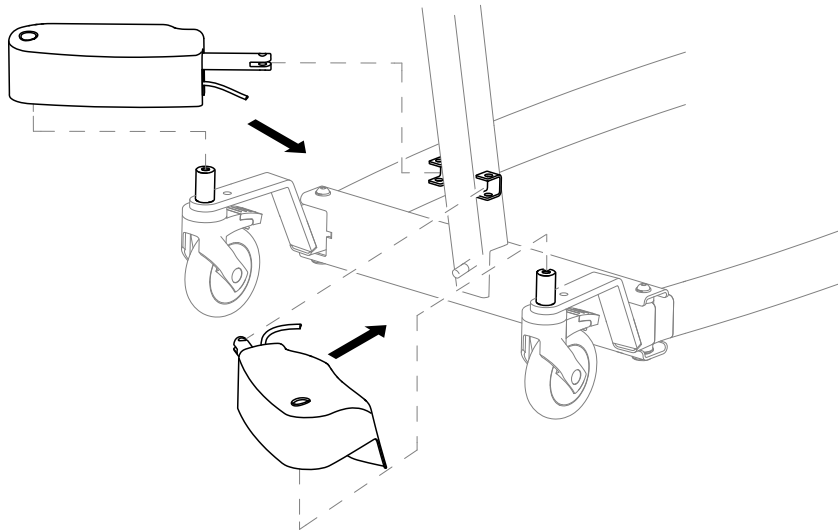



6.

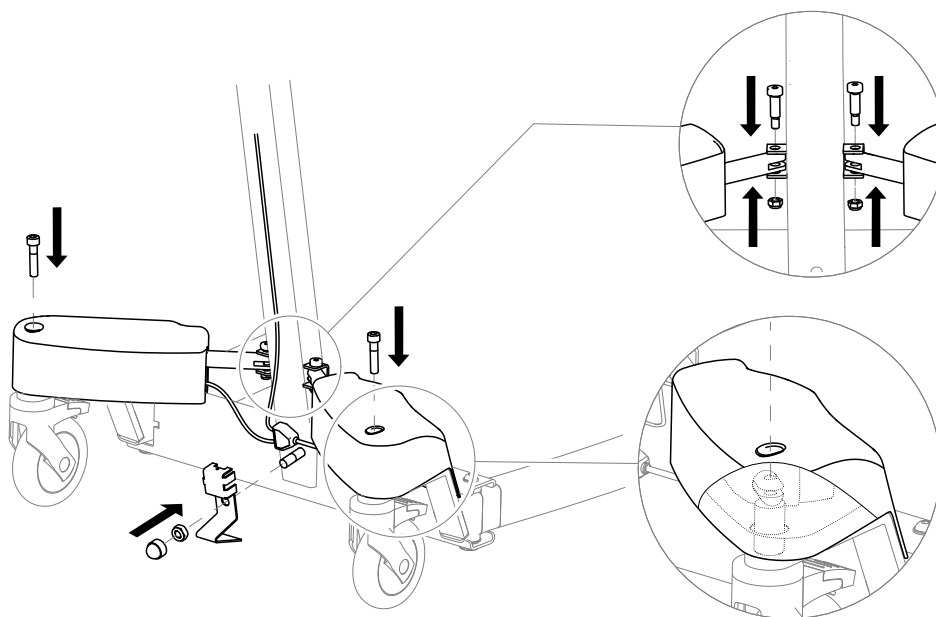


5.14 Replacing electrical legs without actuator cover

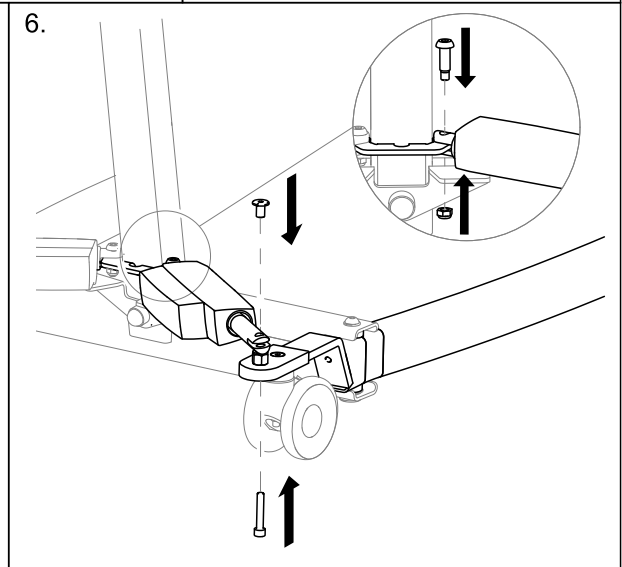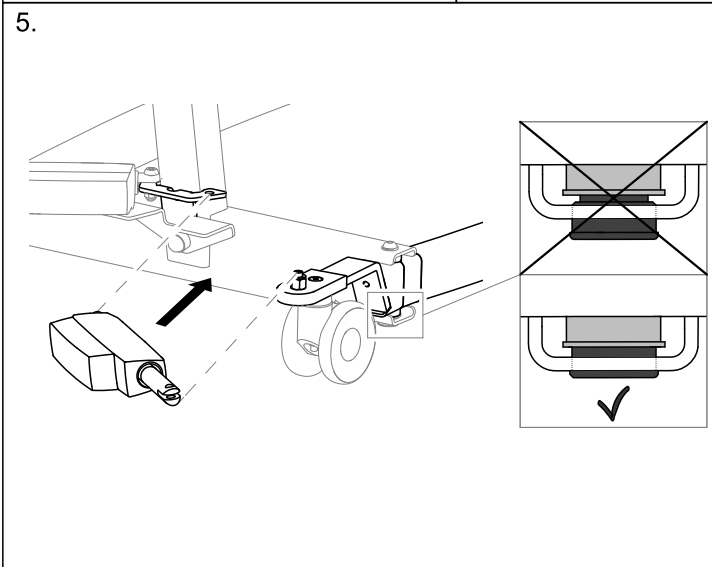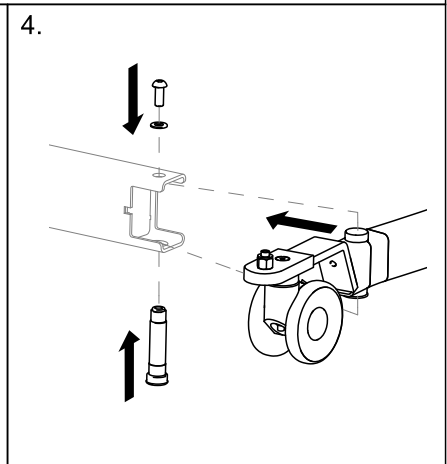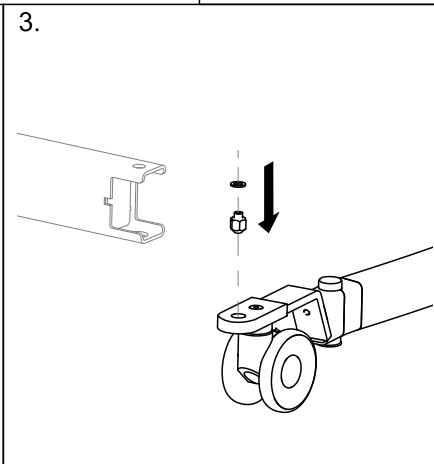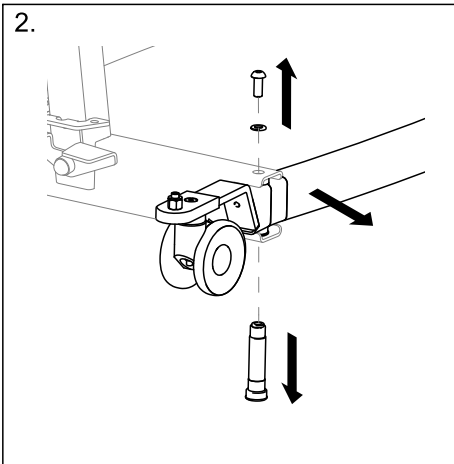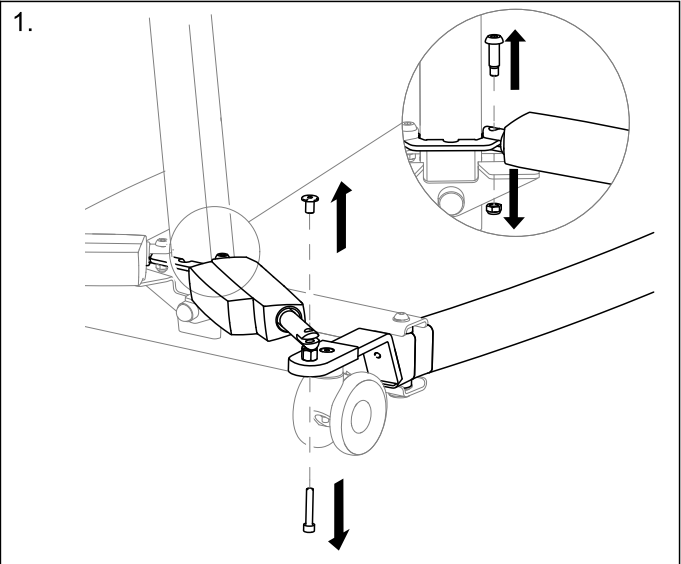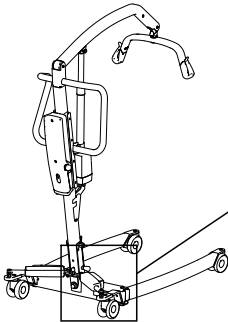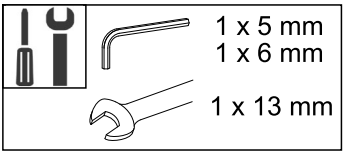


5.15 Replacing electrical legs with actuator cover

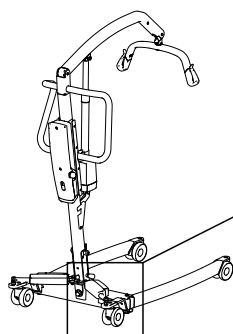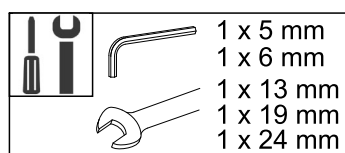


1.

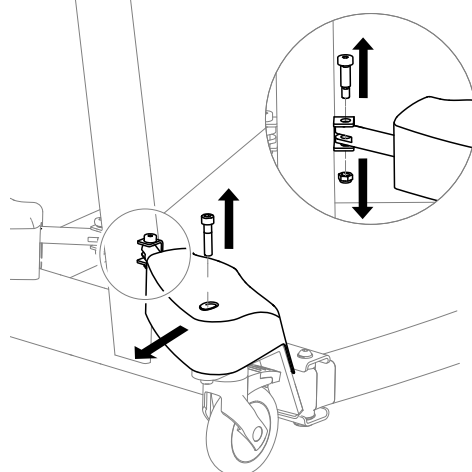


2.

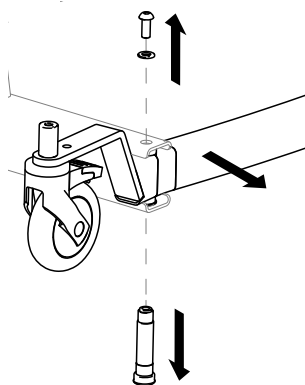


3.

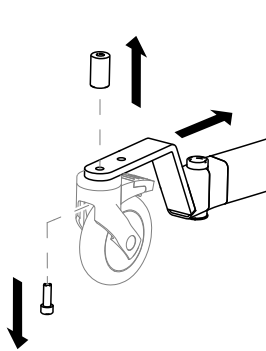


4.

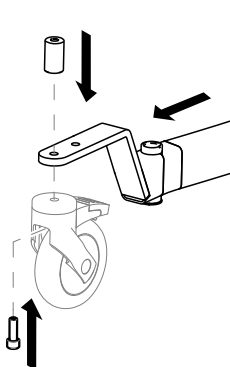


5.

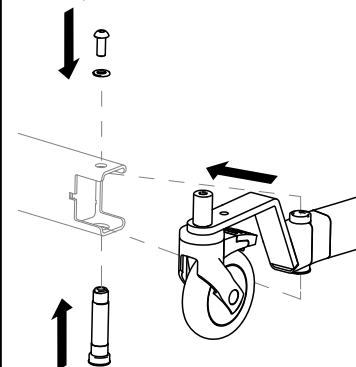


6.

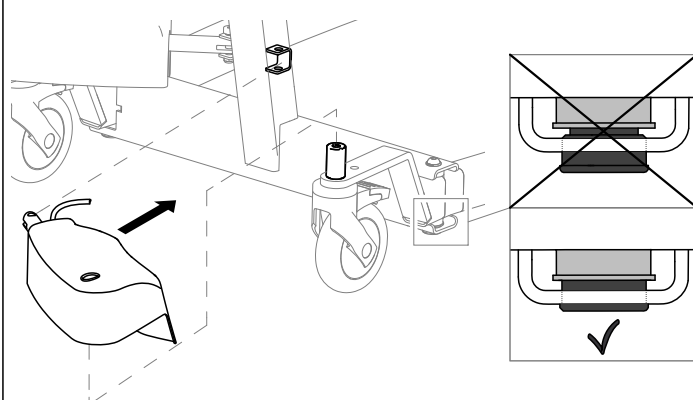




7.

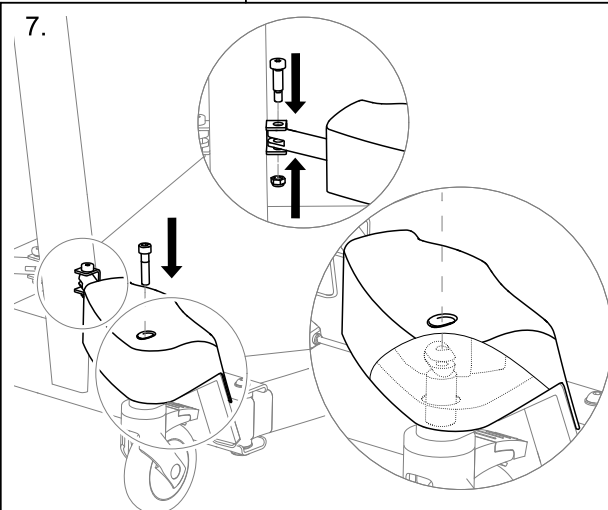




5.16 Replacing the foot pedal and/or rods

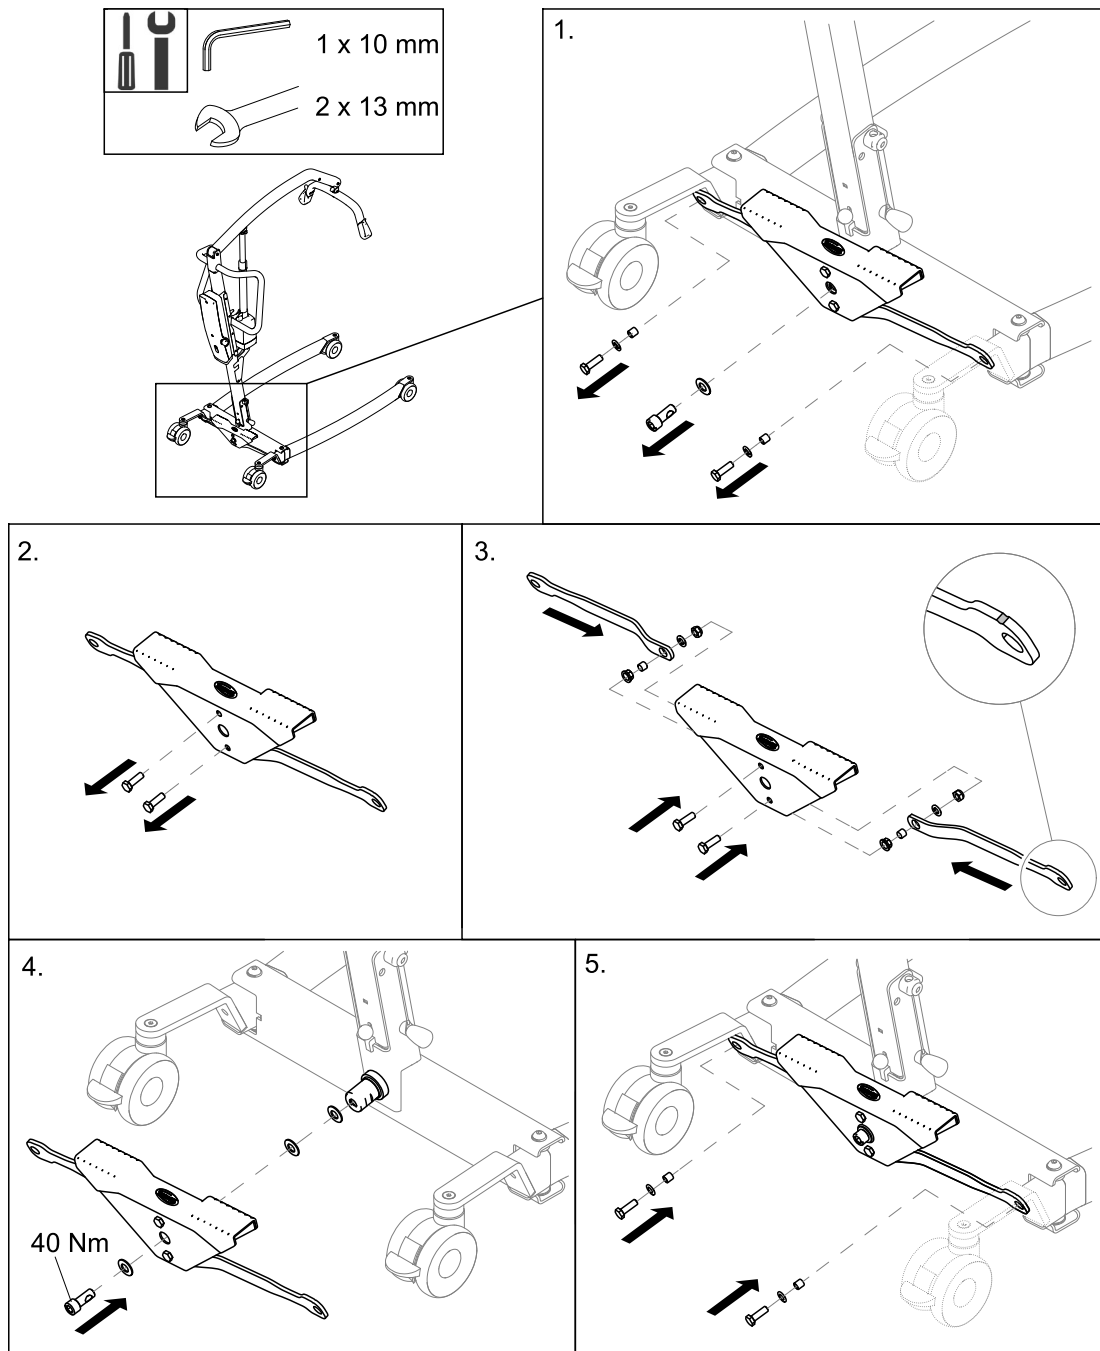



5.17 Replacing manual legs

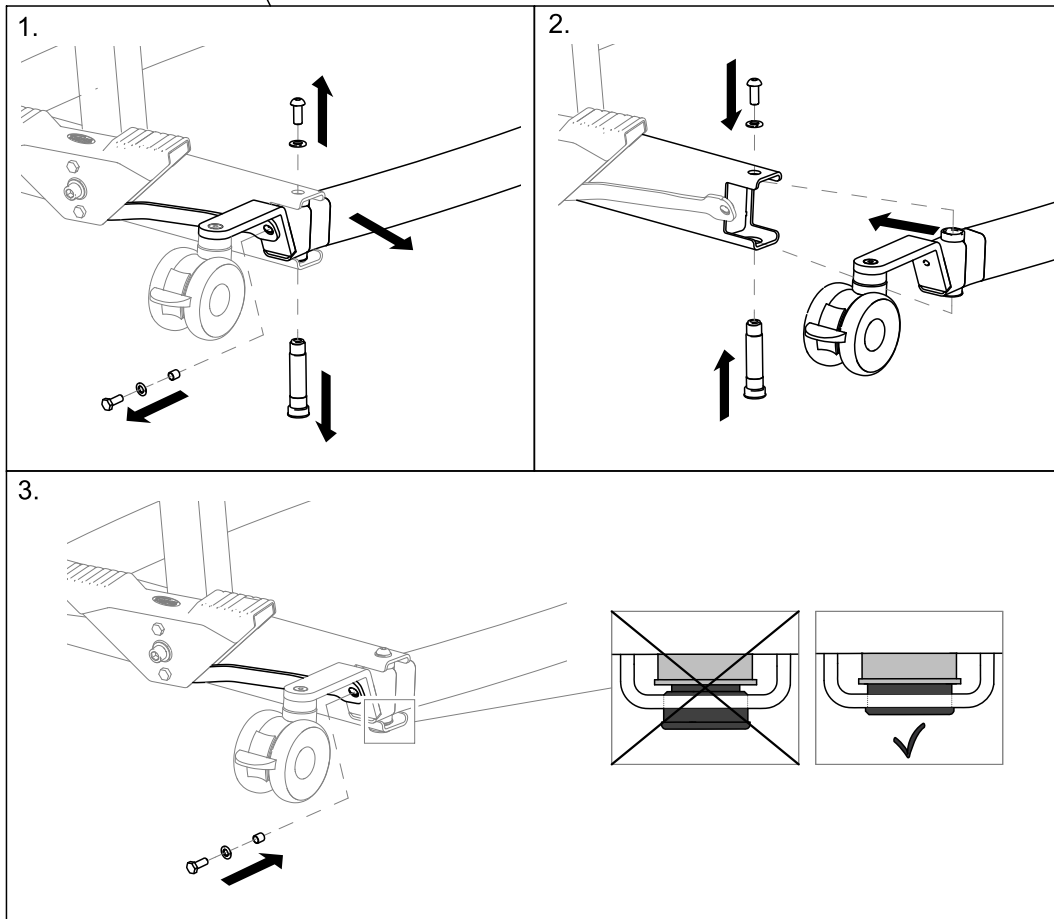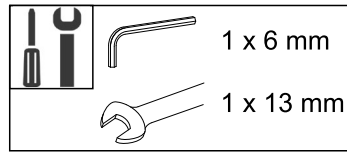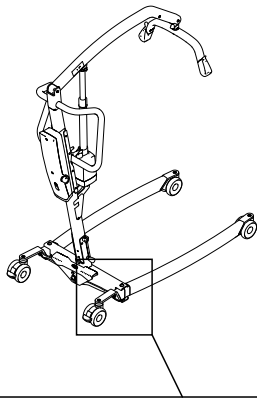


5.18 Replacing the CBJ Home control unit

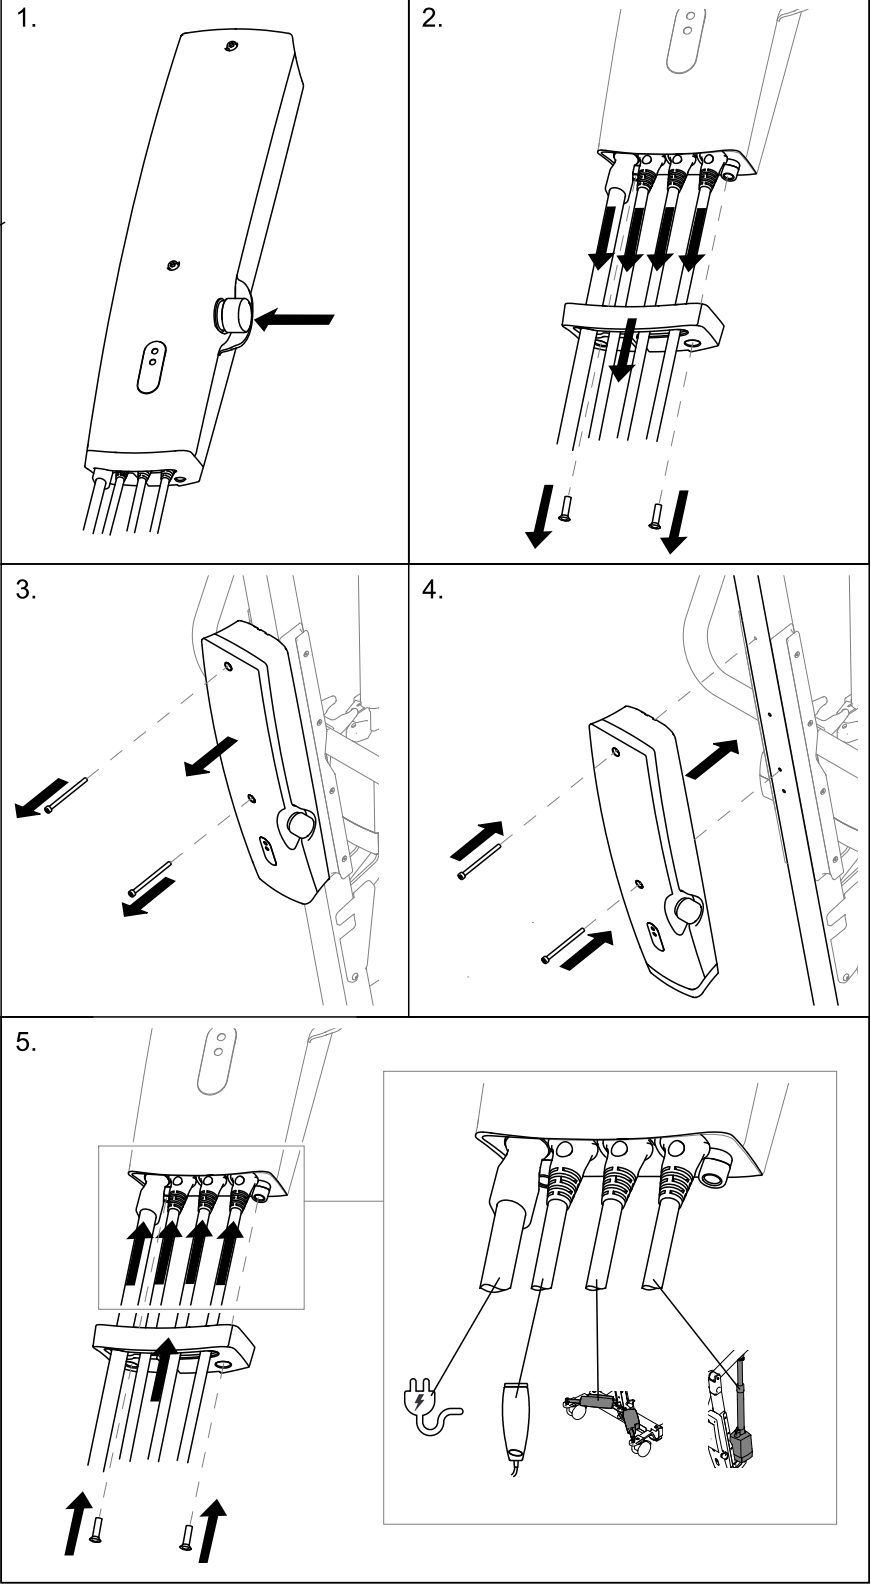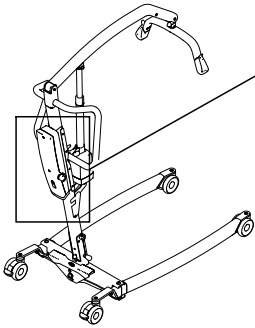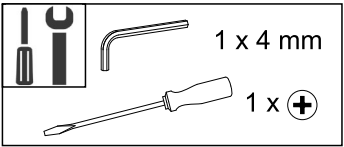


5.19 Replacing the CBJ Care, CBJ1 , CBJ2 control unit

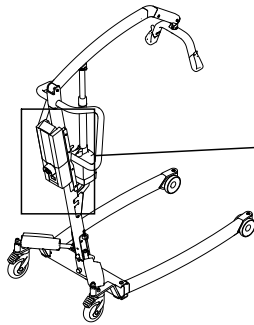


1.

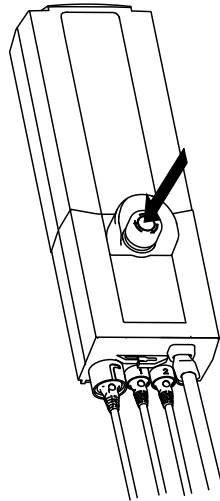


2.

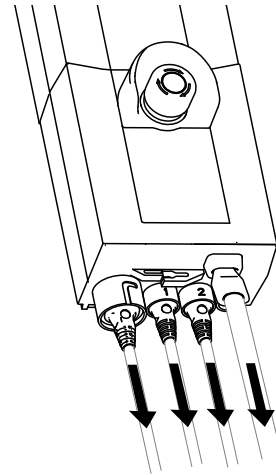


3.

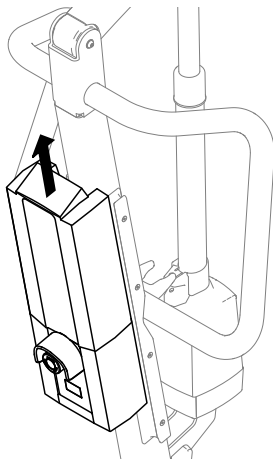


4.

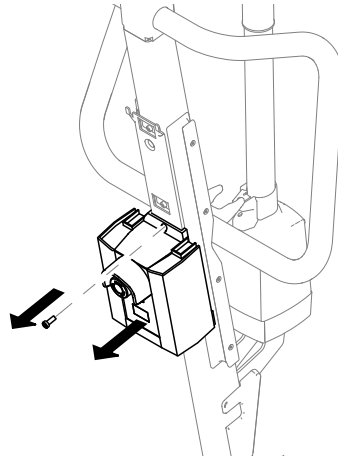


5.

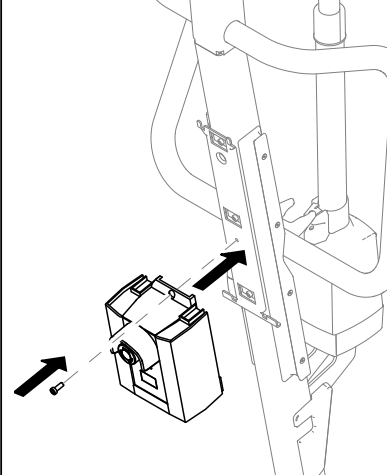










6.

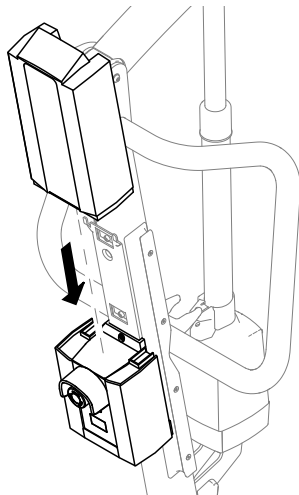


7.

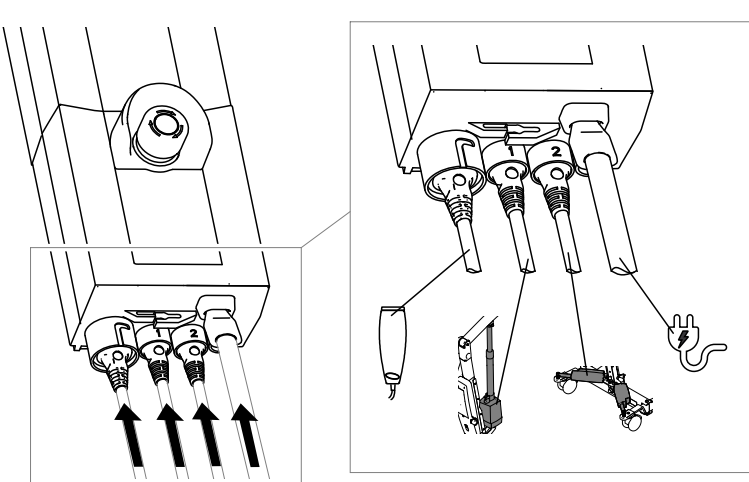


5.20 Installing the Wunder RS300 scale with SMARTLOCK®

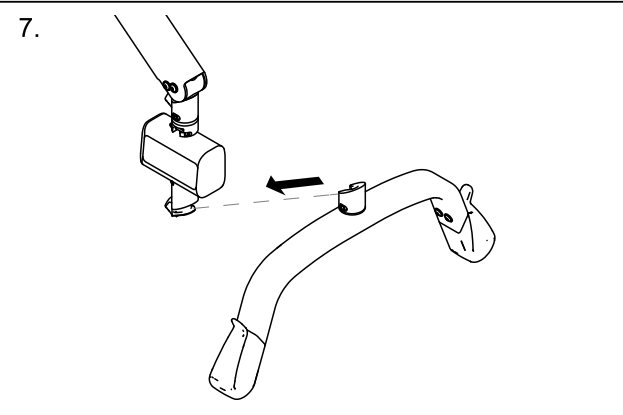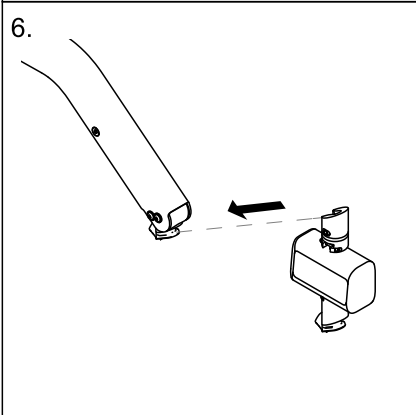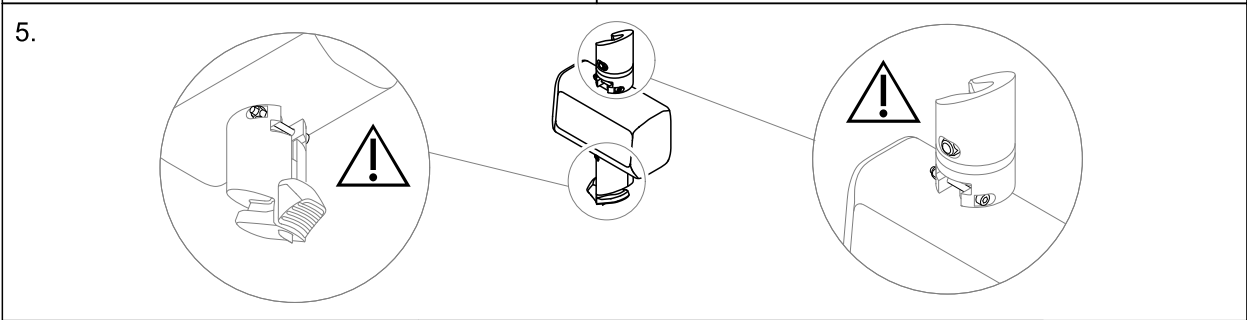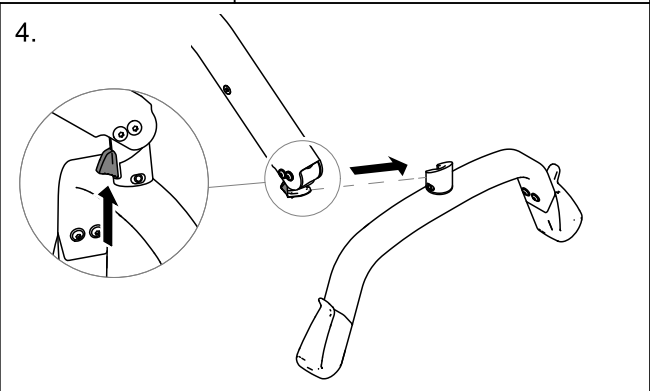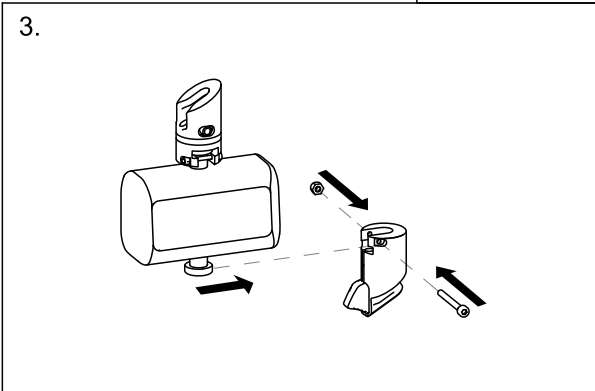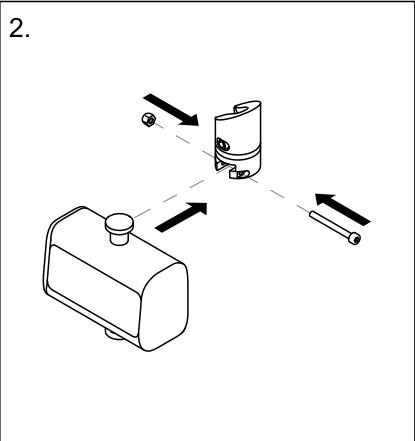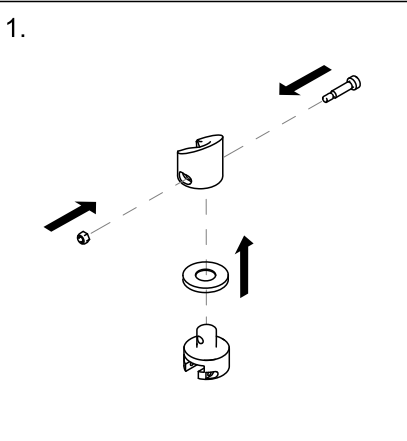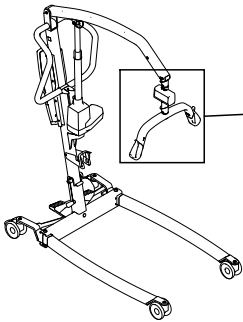


5.21 Installing the Wunder RS300 scale with a fixed spreader bar

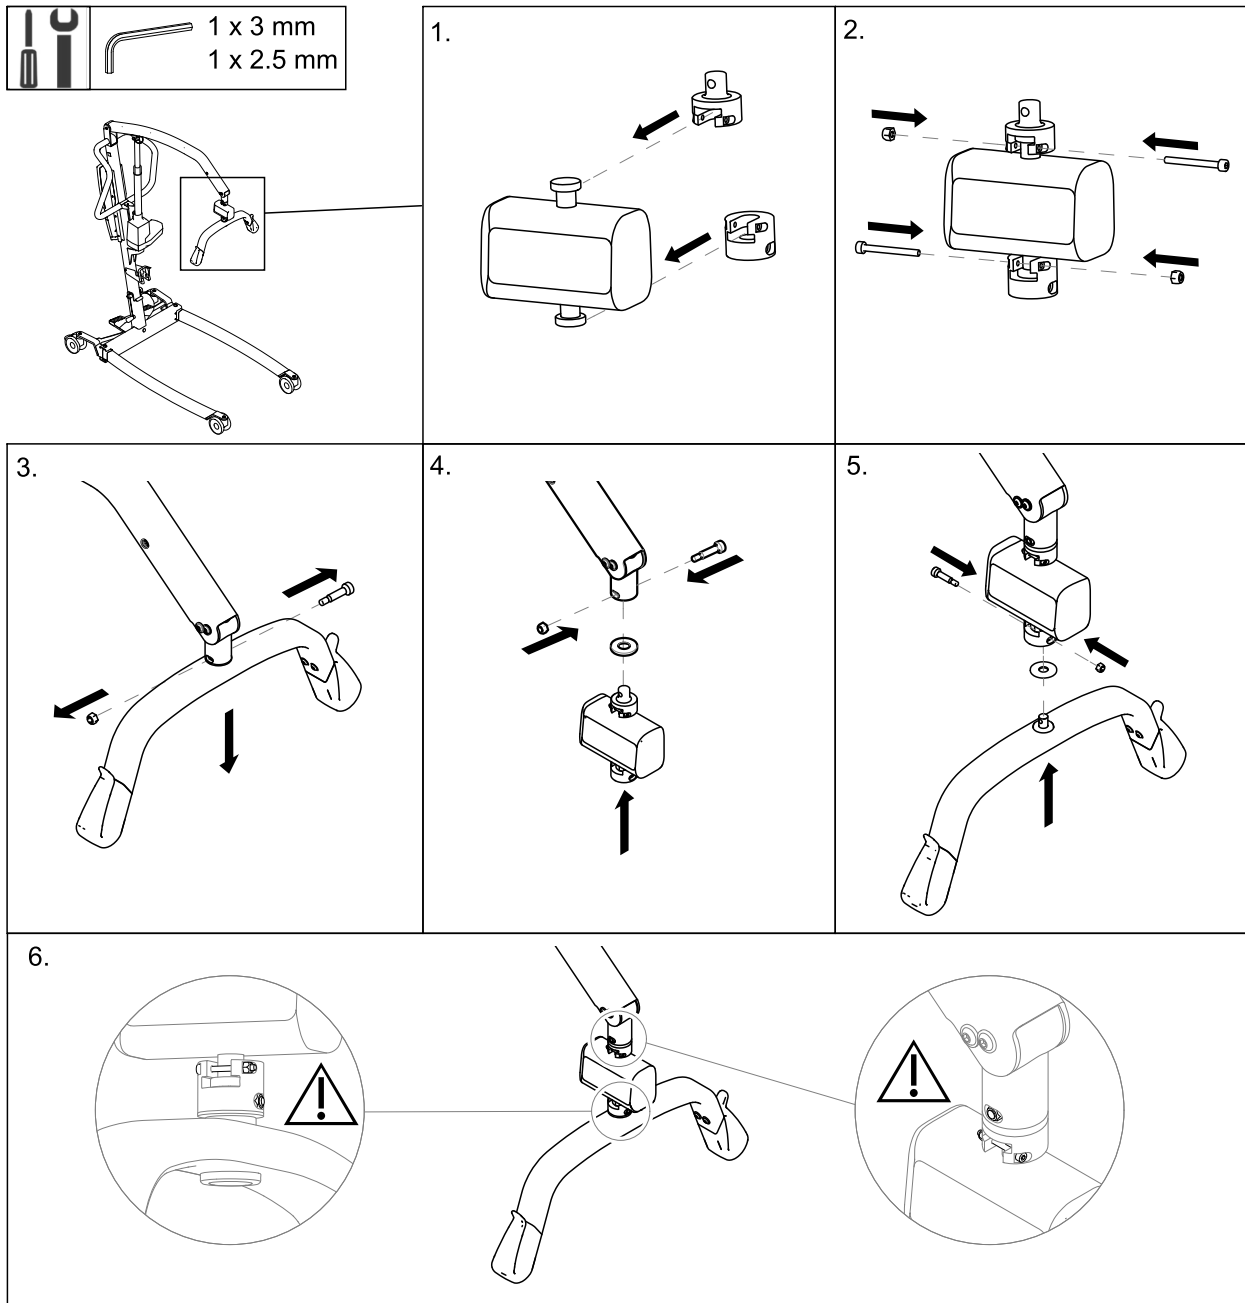





5.22 Installing the Wunder CR200 scale with SMARTLOCK®

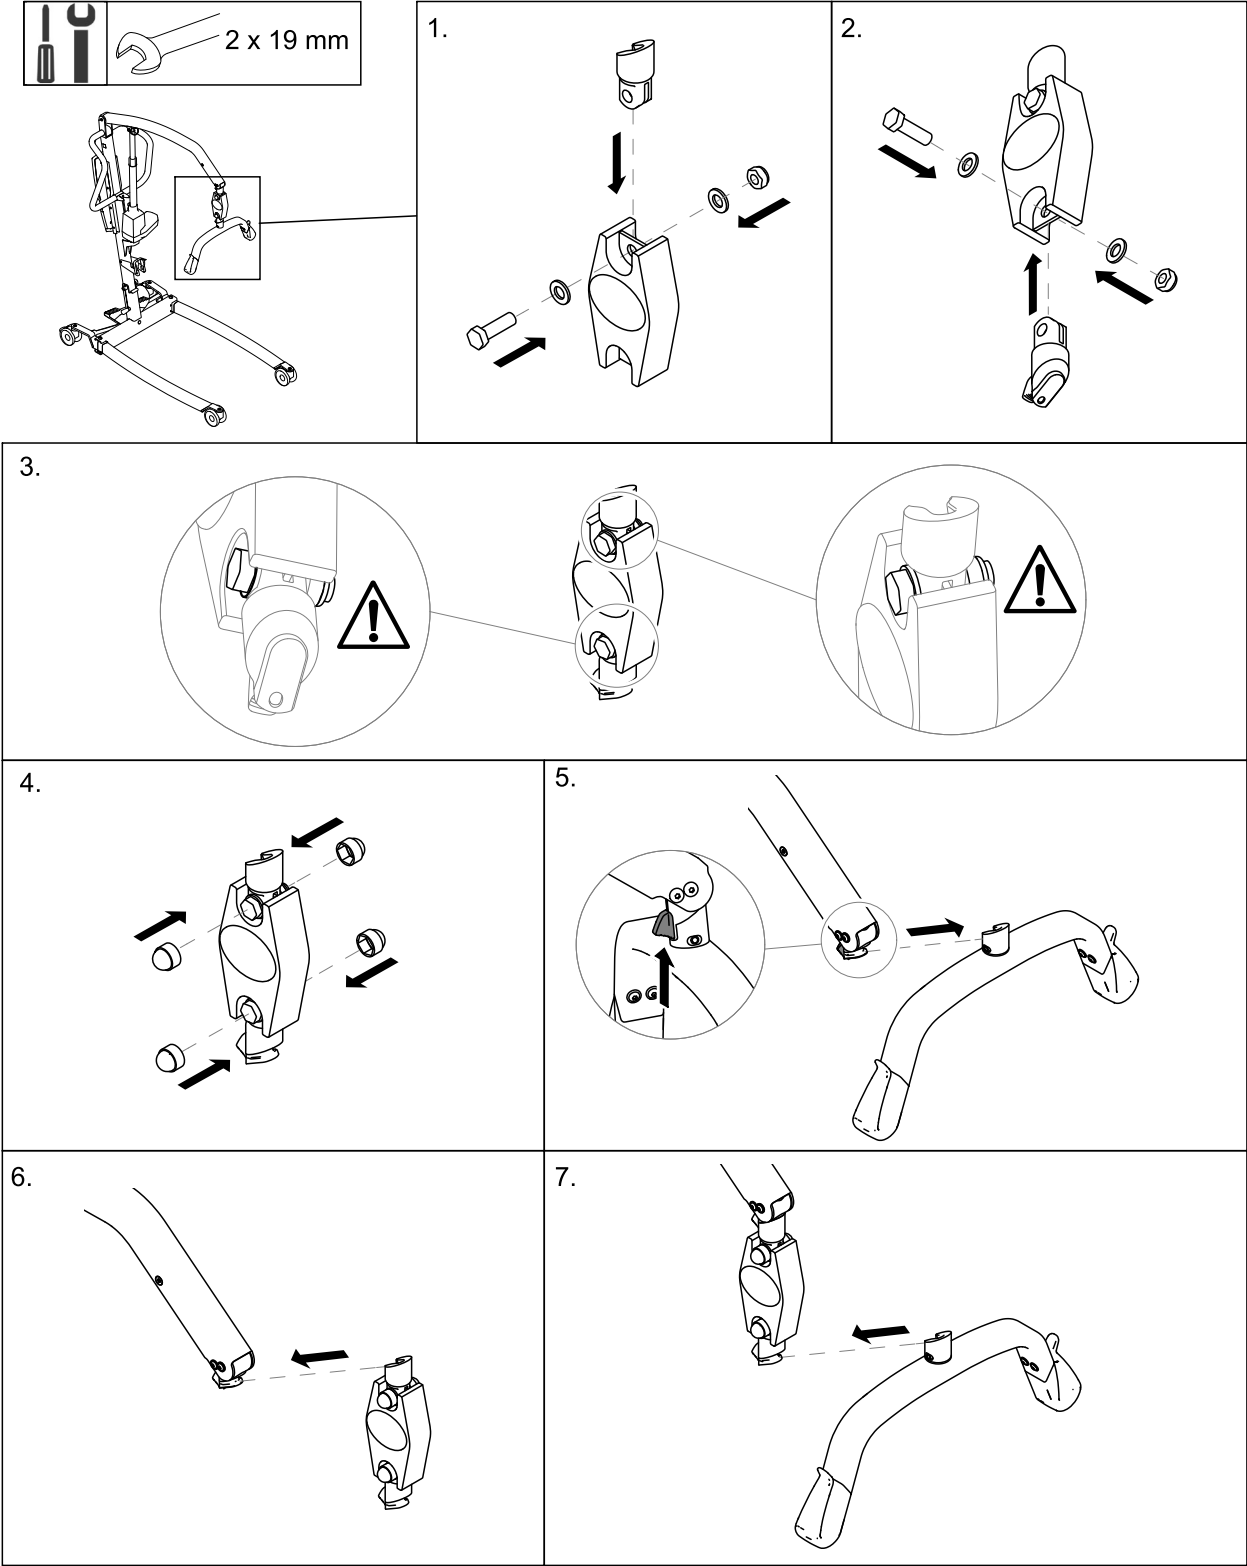

5.23 Installing the Wunder CR200 scale with a fixed spreader bar

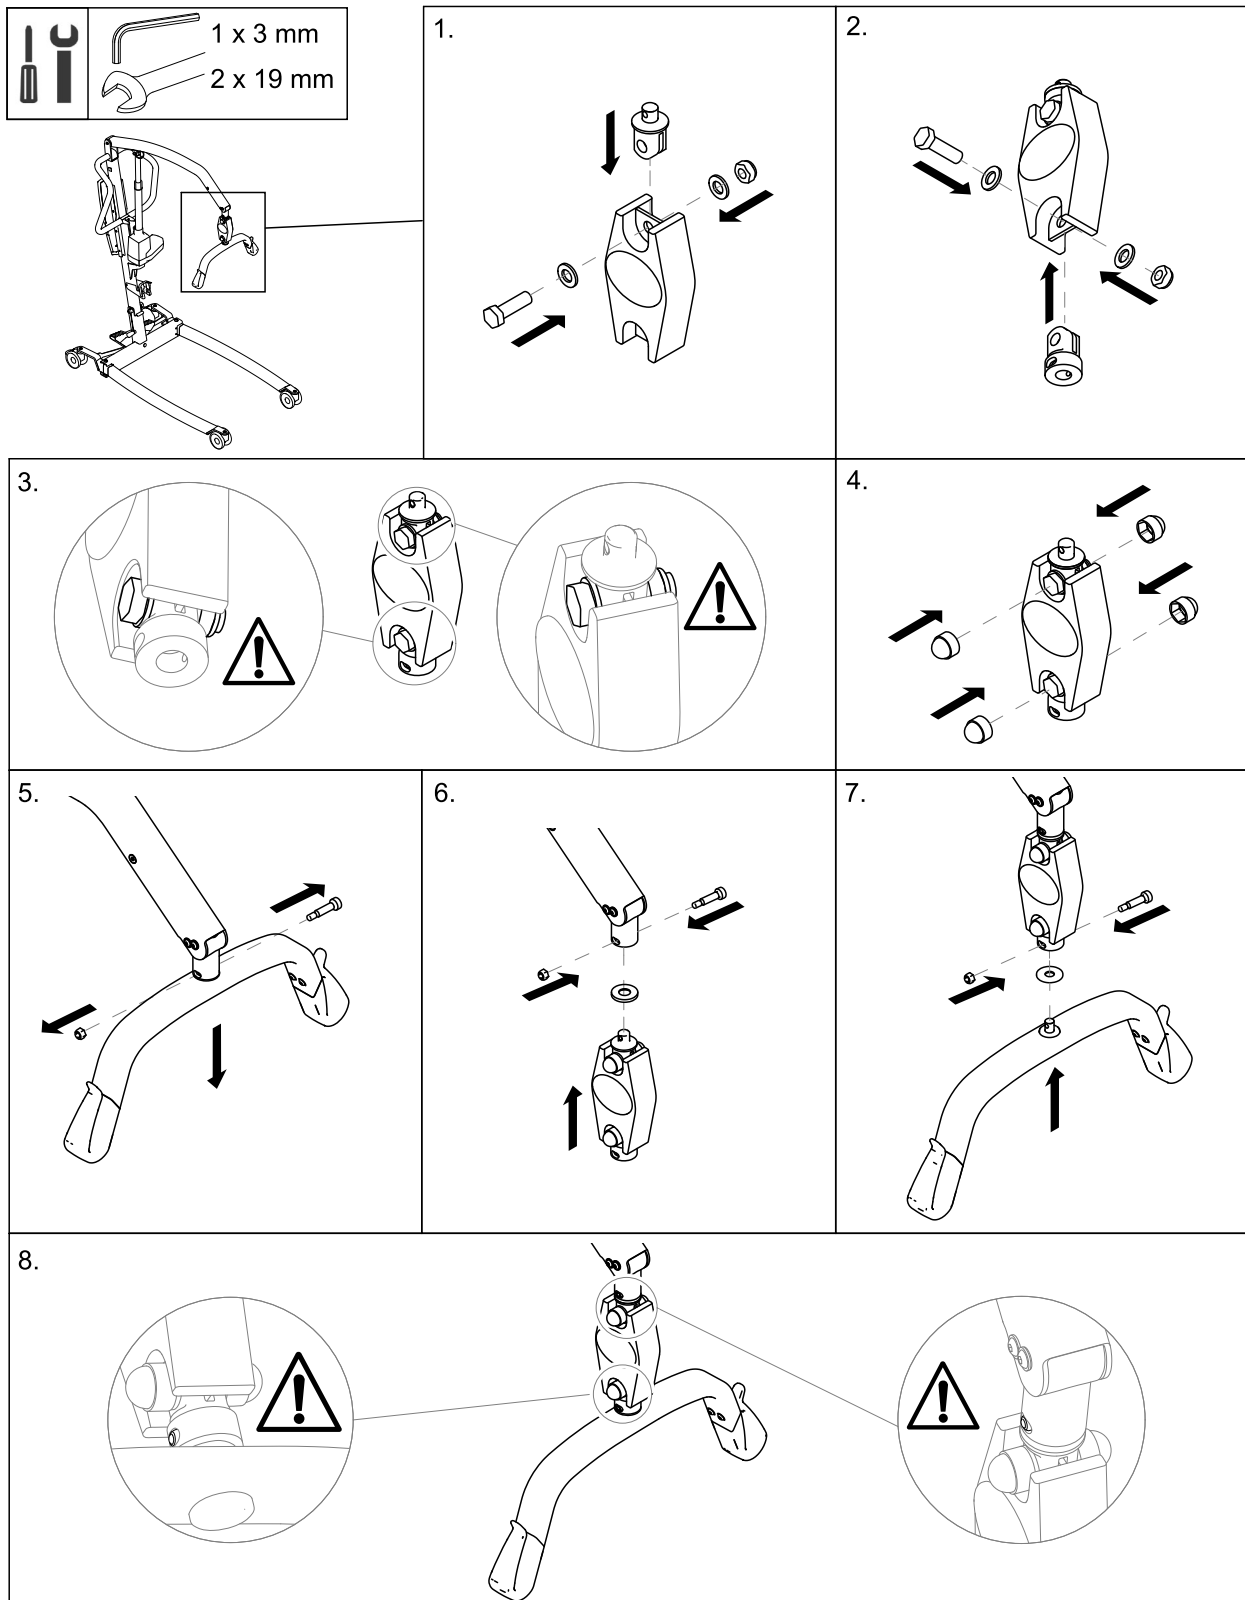

5.24 Installing the lever for manual leg spreader

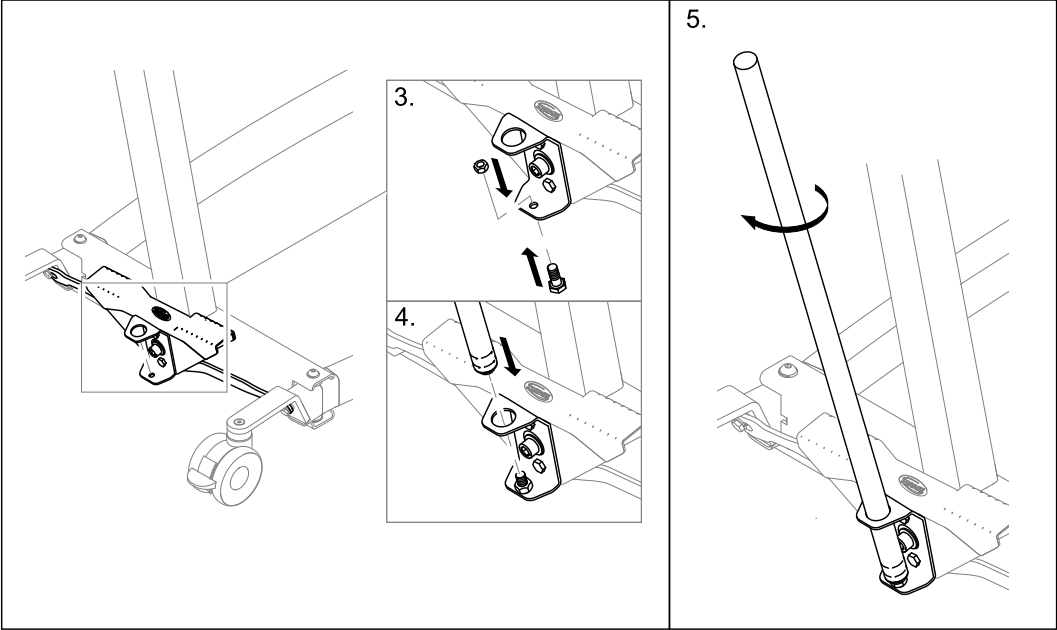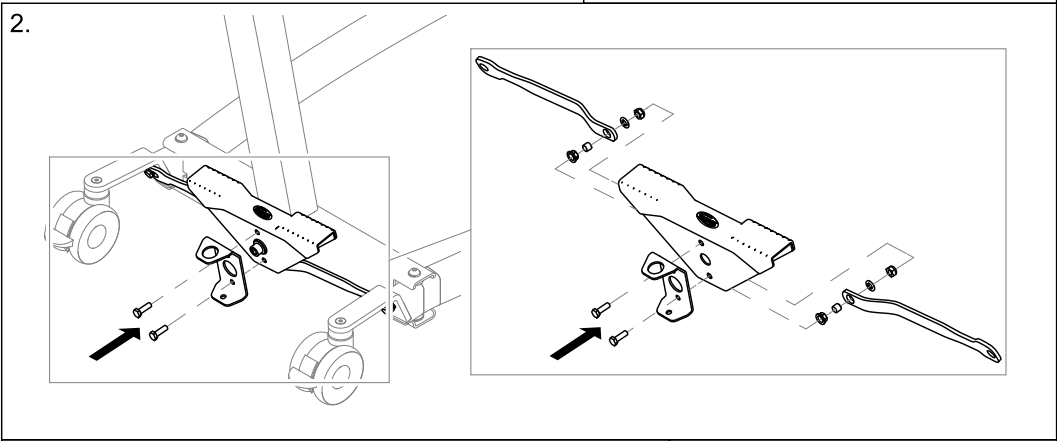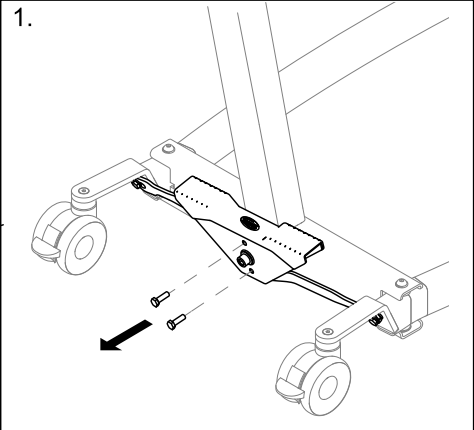

Invacare Distributors

Ireland:

Invacare Ireland Ltd,
Unit 5 Seatown Business Campus
Seatown Road, Swords, County
Dublin
Tel : (353) 1 810 7084
Fax: (353) 1 810 7085
ireland@invacare.com
www.invacare.ie

United Kingdom:

Invacare Limited
Pencoed Technology Park, Pencoed
Bridgend CF35 5AQ
Tel: (44) (0) 1656 776 222
Fax: (44) (0) 1656 776 220
uk@invacare.com
www.invacare.co.uk

Danmark:

Invacare A/S
Sdr. Ringvej 37
DK-2605 Brøndby
Tel: (45) (0)36 90 00 00
Fax: (45) (0)36 90 00 01
denmark@invacare.com
www.invacare.dk

Deutschland:

Invacare GmbH
Am Achener Hof 8
D-88316 Isny
Tel: (49) (0)7562 700 0
kontakt@invacare.com
www.invacare.de

Österreich:

Invacare Austria GmbH
Herzog-Odilo-Straße 101
A-5310 Mondsee-Tiefgraben
Tel: (43) 6232 5535 0
Fax: (43) 6232 5535 4
info-austria@invacare.com
www.invacare.at

Schweiz / Suisse / Svizzera:

Invacare AG
Benkenstrasse 260
CH-4108 Witterswil
Tel: (41) (0)61 487 70 80
Fax: (41) (0)61 487 70 81
switzerland@invacare.com
www.invacare.ch

España:

Invacare SA
Avda. Del Oeste n.50, 1ª, 1ª
Valencia-46001
Tel: (34) (0)972 49 32 14
contactsp@invacare.com
www.invacare.es

France:

Invacare Poirier SAS
Route de St Roch
F-37230 Fondettes
Tel: (33) (0)2 47 62 64 66
Fax: (33) (0)2 47 42 12 24
contactfr@invacare.com
www.invacare.fr

Italia:

Invacare Mecc San s.r.l.,
Via dei Pini 62,
I-36016 Thiene (VI)
Tel: (39) 0445 38 00 59
Fax: (39) 0445 38 00 34
italia@invacare.com
www.invacare.it

Nederland:

Invacare BV
Galvanistraat 14-3
NL-6716 AE Ede
Tel: (31) (0)318 695 757
Fax: (31) (0)318 695 758
nederland@invacare.com
www.invacare.nl

Belgium & Luxemburg:

Invacare nv
Autobaan 22
B-8210 Loppem
Tel: (32) (0)50 83 10 10
Fax: (32) (0)50 83 10 11
belgium@invacare.com
www.invacare.be

Norge:

Invacare AS
Grensesvingen 9, Postboks 6230,
Etterstad
N-0603 Oslo
Tel: (47) (0)22 57 95 00
Fax: (47) (0)22 57 95 01
norway@invacare.com
www.invacare.no

Portugal:

Invacare Lda
Rua Estrada Velha, 949
P-4465-784 Leça do Balio
Tel: (351) (0)225 193 360
Fax: (351) (0)225 1057 39
portugal@invacare.com
www.invacare.pt

Suomi:

Camp Mobility
Patamäenkatu 5, 33900 Tampere
Puhelin 09-35076310
info@campmobility.fi
www.campmobility.fi

Sverige:

Invacare AB
Fagerstagatan 9
S-163 53 Spånga
Tel: (46) (0)8 761 70 90
Fax: (46) (0)8 761 81 08
sweden@invacare.com
www.invacare.se

Australia:

Invacare Australia Pty. Ltd.
1 Lenton Place, North Rocks NSW
2151
Australia
Phone: 1800 460 460
Fax: 1800 814 367
orders@invacare.com.au
www.invacare.com.au

New Zealand:

Invacare New Zealand Ltd
4 Westfield Place, Mt Wellington
1060
New Zealand
Phone: 0800 468 222
Fax: 0800 807 788
sales@invacare.co.nz
www.invacare.co.nz



Invacare Portugal, Lda
Rua Estrada Velha 949
4465-784 Leça do Balio
Portugal

